




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052523\
 Data File : VV031238.D
 Acq On : 25 May 2023 17:34
 Operator : SY/MD
 Sample : VV0525WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK341

Manual IntegrationsAPPROVED

Quant Time: May 26 07:02:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052523WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri May 26 06:48:38 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/26/2023
 Supervised By :Mahesh Dadoda 05/26/2023

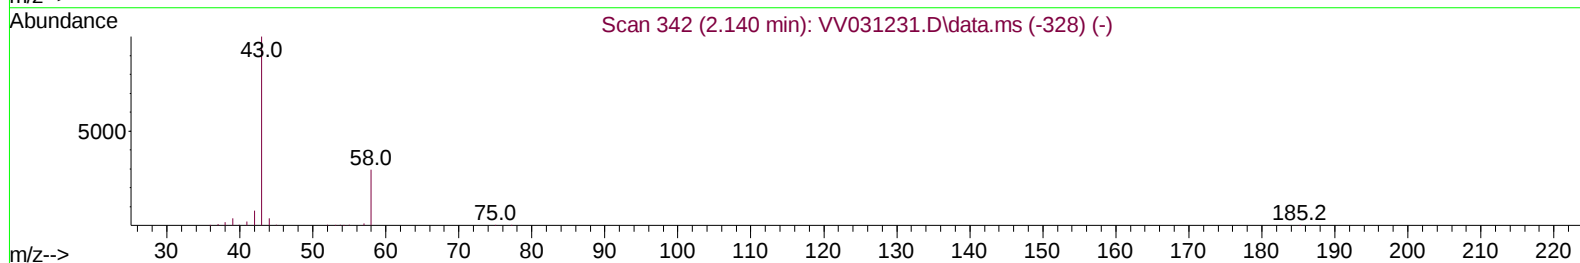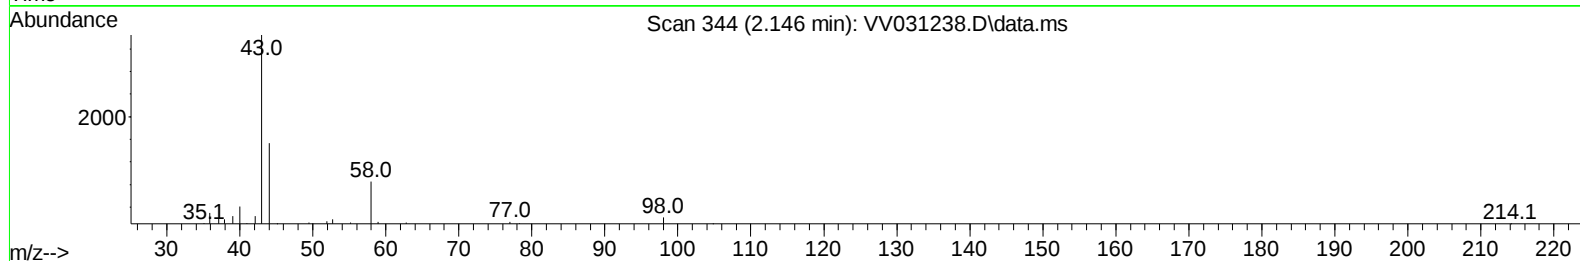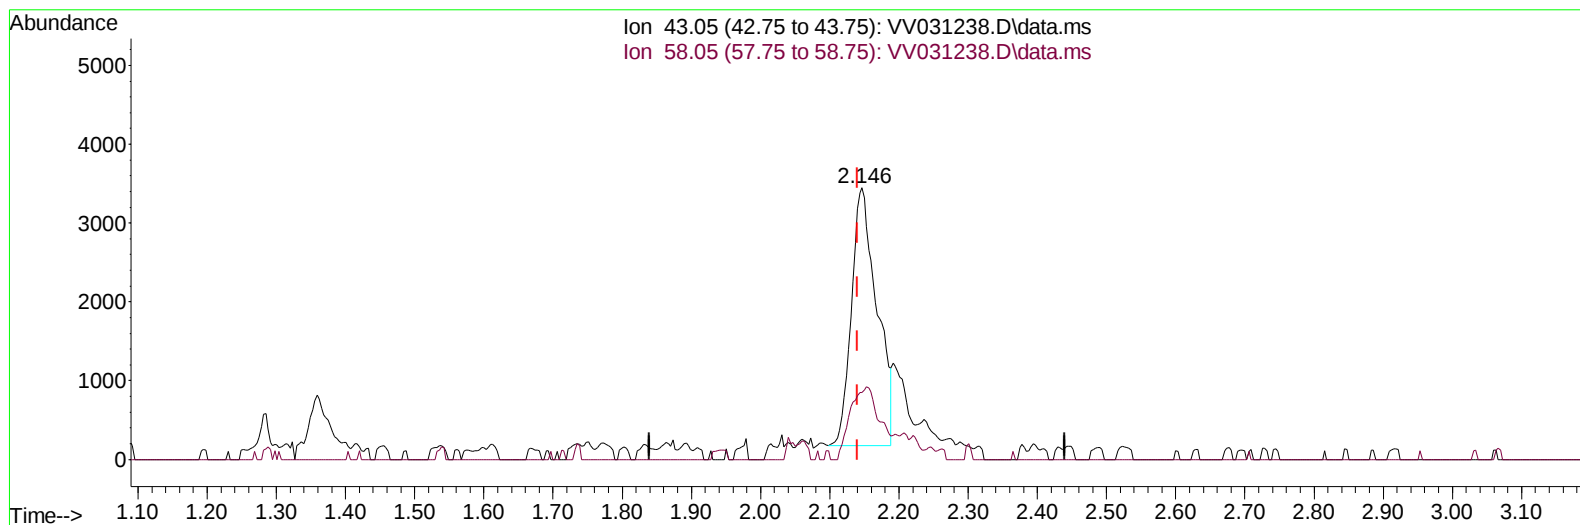

TIC: VV031238.D\data.ms

(13) Acetone (T)

2.146min (+ 0.007) 3.56 ug/L

response 8390

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	31.10	32.35
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052523\
 Data File : VV031238.D
 Acq On : 25 May 2023 17:34
 Operator : SY/MD
 Sample : VV0525WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK341

Manual IntegrationsAPPROVED

Quant Time: May 26 07:02:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052523WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri May 26 06:48:38 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/26/2023
 Supervised By :Mahesh Dadoda 05/26/2023

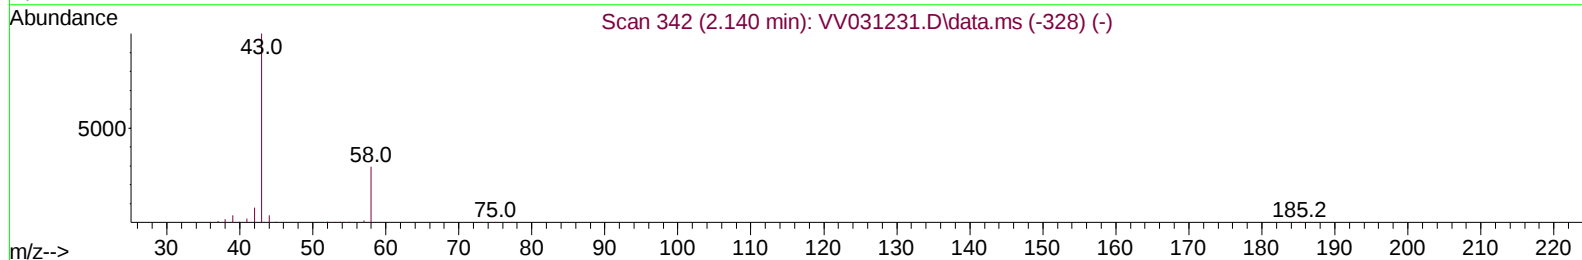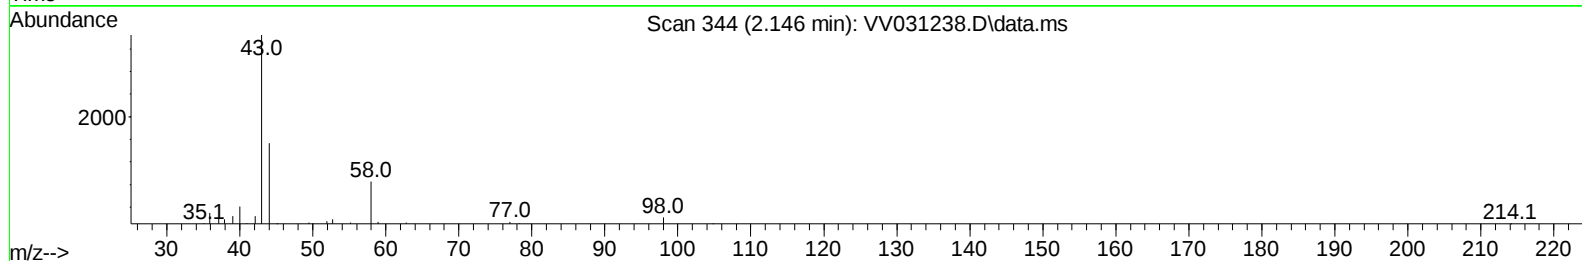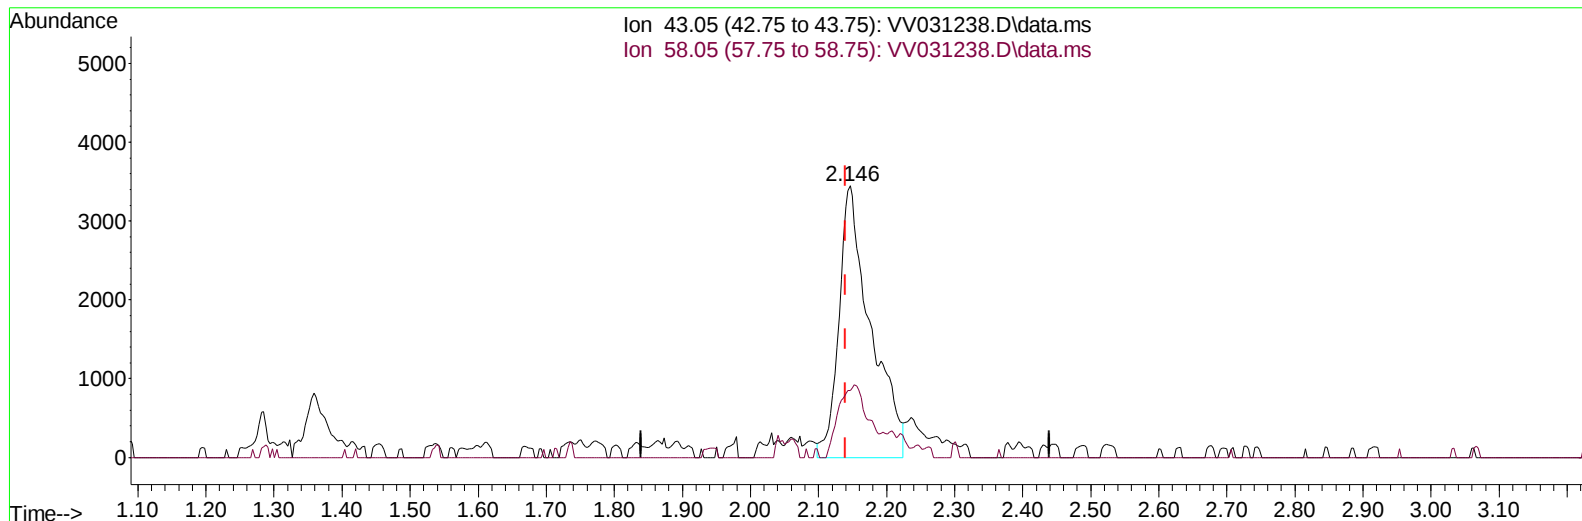

TIC: VV031238.D\data.ms

(13) Acetone (T)

2.146min (+ 0.007) 4.71 ug/L m

response 11089

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	31.10	24.47
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052523\
 Data File : VV031238.D
 Acq On : 25 May 2023 17:34
 Operator : SY/MD
 Sample : VV0525WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK341

Manual IntegrationsAPPROVED

Quant Time: May 26 07:02:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052523WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri May 26 06:48:38 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/26/2023
 Supervised By :Mahesh Dadoda 05/26/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.542	114		125670	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117		122102	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		53807	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.282	65		75372	5.412	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	108.200%	
7) Chloroethane-d5	1.536	69		60383	5.558	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	111.200%	
11) 1,1-Dichloroethene-d2	2.063	65		35178	6.111	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	122.200%	
20) 2-Butanone-d5	3.815	46		190319	63.488	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	126.980%	
24) Chloroform-d	4.259	84		154112	5.580	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	111.600%	
26) 1,2-Dichloroethane-d4	4.950	65		81132	5.945	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	119.000%	
32) Benzene-d6	4.969	84		267737	5.251	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	105.000%	
36) 1,2-Dichloropropane-d6	5.995	67		86573	5.074	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	101.400%	
41) Toluene-d8	7.249	98		187773	4.214	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	84.200%	
43) trans-1,3-Dichloroprop...	7.561	79		25113	4.577	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	91.600%	
46) 2-Hexanone-d5	8.034	63		118568	52.929	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	105.860%	
56) 1,1,2,2-Tetrachloroeth...	10.159	84		59477	4.939	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	98.800%	
66) 1,2-Dichlorobenzene-d4	11.567	152		63721	5.048	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	101.000%	
Target Compounds							
13) Acetone	2.146	43		11089m	4.707	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052523\
Data File : VV031238.D
Acq On : 25 May 2023 17:34
Operator : SY/MD
Sample : VV0525WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
VBLK341

Manual IntegrationsAPPROVED

Quant Time: May 26 07:02:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052523WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri May 26 06:48:38 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 05/26/2023
Supervised By :Mahesh Dadoda 05/26/2023

