




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052523\
 Data File : VV031239.D
 Acq On : 25 May 2023 17:59
 Operator : SY/MD
 Sample : 02917-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C11G5

Manual IntegrationsAPPROVED

Quant Time: May 26 07:02:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052523WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri May 26 06:48:38 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/26/2023
 Supervised By :Mahesh Dadoda 05/26/2023

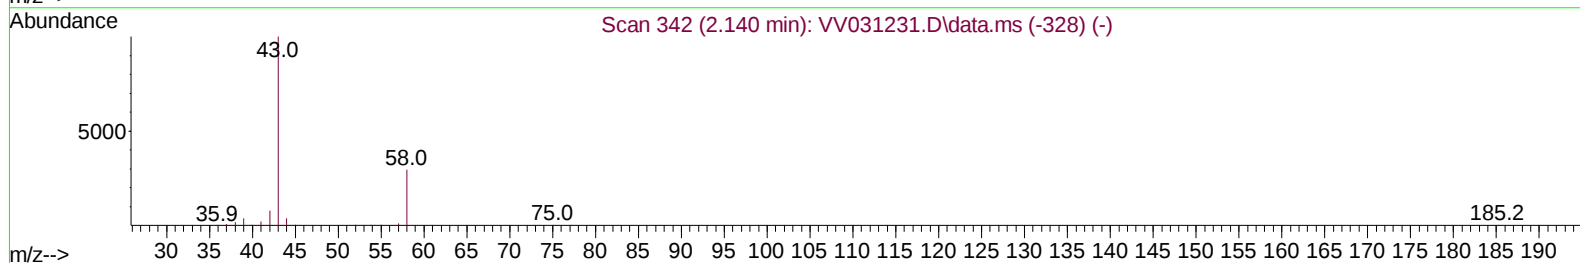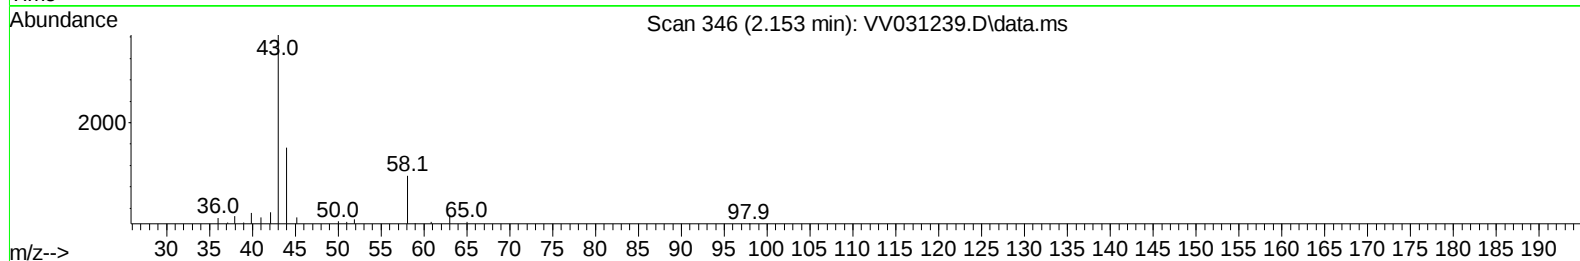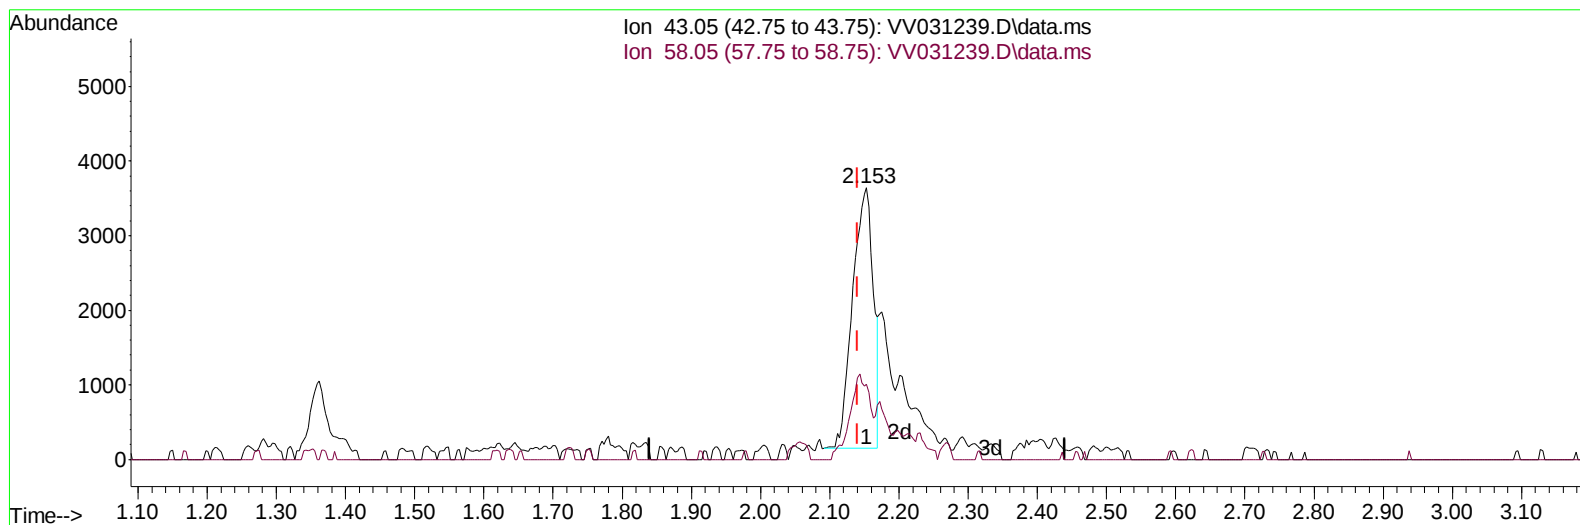

TIC: VV031239.D\data.ms

(13) Acetone (T)

2.153min (+ 0.013) 2.68 ug/L

response 7263

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	31.10	31.02
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052523\
 Data File : VV031239.D
 Acq On : 25 May 2023 17:59
 Operator : SY/MD
 Sample : 02917-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C11G5

Manual IntegrationsAPPROVED

Quant Time: May 26 07:02:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052523WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri May 26 06:48:38 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/26/2023
 Supervised By :Mahesh Dadoda 05/26/2023

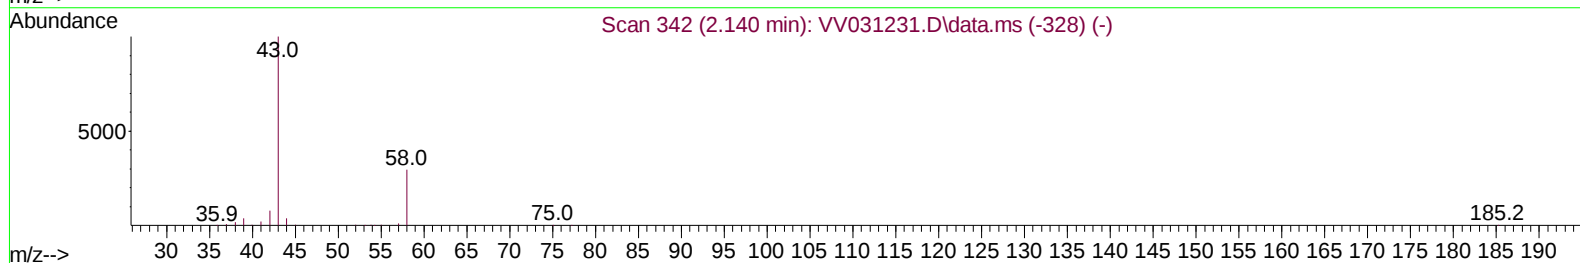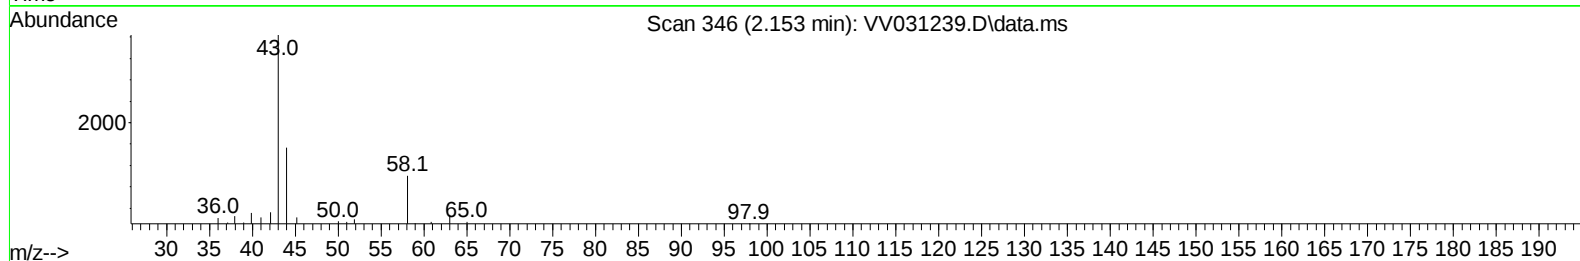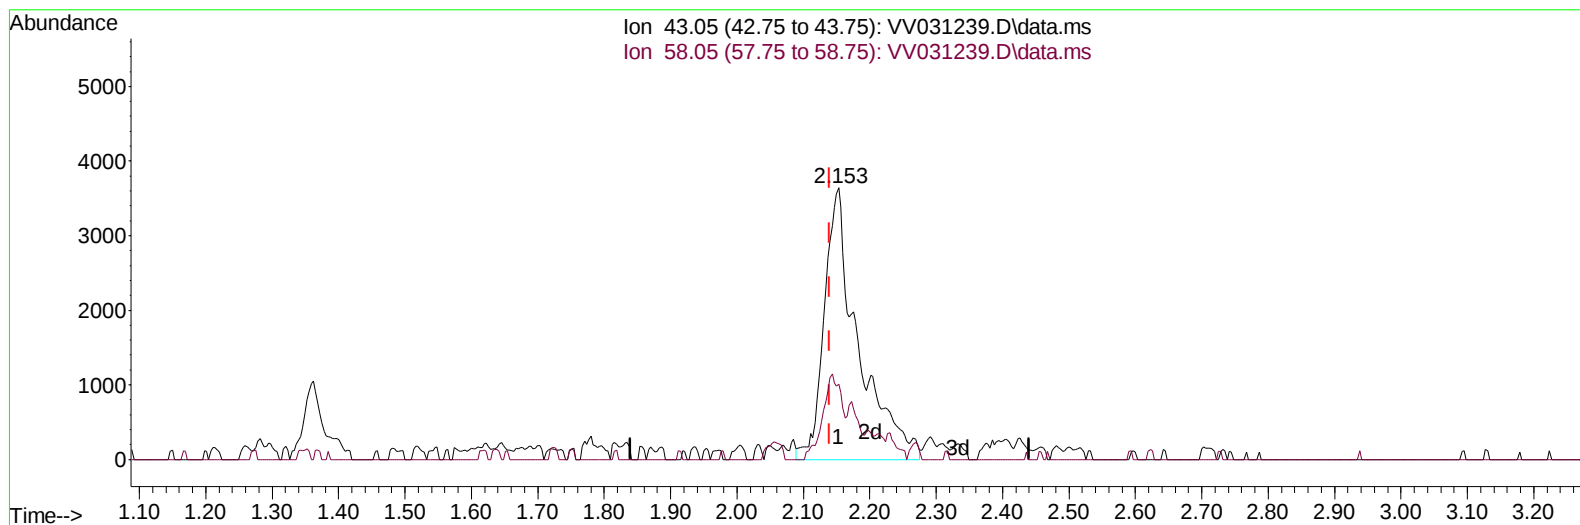

TIC: VV031239.D\data.ms

(13) Acetone (T)

2.153min (+ 0.013) 4.75 ug/L m

response 12891

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	31.10	17.48
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052523\
 Data File : VV031239.D
 Acq On : 25 May 2023 17:59
 Operator : SY/MD
 Sample : 02917-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C11G5

Manual IntegrationsAPPROVED

Quant Time: May 26 07:02:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052523WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri May 26 06:48:38 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/26/2023
 Supervised By :Mahesh Dadoda 05/26/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.542	114		144789	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117		135003	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		64434	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.282	65		75906	4.730	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	94.600%		
7) Chloroethane-d5	1.536	69		61852	4.941	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	98.800%		
11) 1,1-Dichloroethene-d2	2.063	65		32404	4.885	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	97.800%		
20) 2-Butanone-d5	3.818	46		184778	53.500	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery =	107.000%		
24) Chloroform-d	4.256	84		154779	4.864	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	97.200%		
26) 1,2-Dichloroethane-d4	4.953	65		80248	5.104	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	102.000%		
32) Benzene-d6	4.970	84		268934	4.770	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	95.400%		
36) 1,2-Dichloropropane-d6	5.995	67		92295	4.892	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	97.800%		
41) Toluene-d8	7.249	98		189184	3.840	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	76.800%		
43) trans-1,3-Dichloroprop...	7.561	79		24389	4.021	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	80.400%		
46) 2-Hexanone-d5	8.034	63		117392	47.396	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	94.800%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84		59064	4.436	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	88.800%		
66) 1,2-Dichlorobenzene-d4	11.567	152		78985	5.225	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	104.400%		
Target Compounds							
13) Acetone	2.153	43		12891m	4.749	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052523\
Data File : VV031239.D
Acq On : 25 May 2023 17:59
Operator : SY/MD
Sample : 02917-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C11G5

Manual IntegrationsAPPROVED

Quant Time: May 26 07:02:16 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052523WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri May 26 06:48:38 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 05/26/2023
Supervised By :Mahesh Dadoda 05/26/2023

