

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052523\
 Data File : VV031239.D
 Acq On : 25 May 2023 17:59
 Operator : SY/MD
 Sample : 02917-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C11G5

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 05/26/2023
 Supervised By :Mahesh Dadoda 05/26/2023

Quant Time: May 26 07:02:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052523WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri May 26 06:48:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	144789	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	135003	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	64434	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	75906	4.730	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	94.600%	
7) Chloroethane-d5	1.536	69	61852	4.941	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	98.800%	
11) 1,1-Dichloroethene-d2	2.063	65	32404	4.885	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	97.800%	
20) 2-Butanone-d5	3.818	46	184778	53.500	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	107.000%	
24) Chloroform-d	4.256	84	154779	4.864	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.200%	
26) 1,2-Dichloroethane-d4	4.953	65	80248	5.104	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.000%	
32) Benzene-d6	4.970	84	268934	4.770	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.400%	
36) 1,2-Dichloropropane-d6	5.995	67	92295	4.892	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.800%	
41) Toluene-d8	7.249	98	189184	3.840	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	76.800%	
43) trans-1,3-Dichloroprop...	7.561	79	24389	4.021	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	80.400%	
46) 2-Hexanone-d5	8.034	63	117392	47.396	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	94.800%	
56) 1,1,2,2-Tetrachloroeth...	10.159	84	59064	4.436	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	88.800%	
66) 1,2-Dichlorobenzene-d4	11.567	152	78985	5.225	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	104.400%	
Target Compounds					Qvalue	
13) Acetone	2.153	43	12891m	4.749	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052523\
Data File : VV031239.D
Acq On : 25 May 2023 17:59
Operator : SY/MD
Sample : 02917-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
C11G5

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 05/26/2023
Supervised By :Mahesh Dadoda 05/26/2023


Quant Time: May 26 07:02:16 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052523WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri May 26 06:48:38 2023
Response via : Initial Calibration

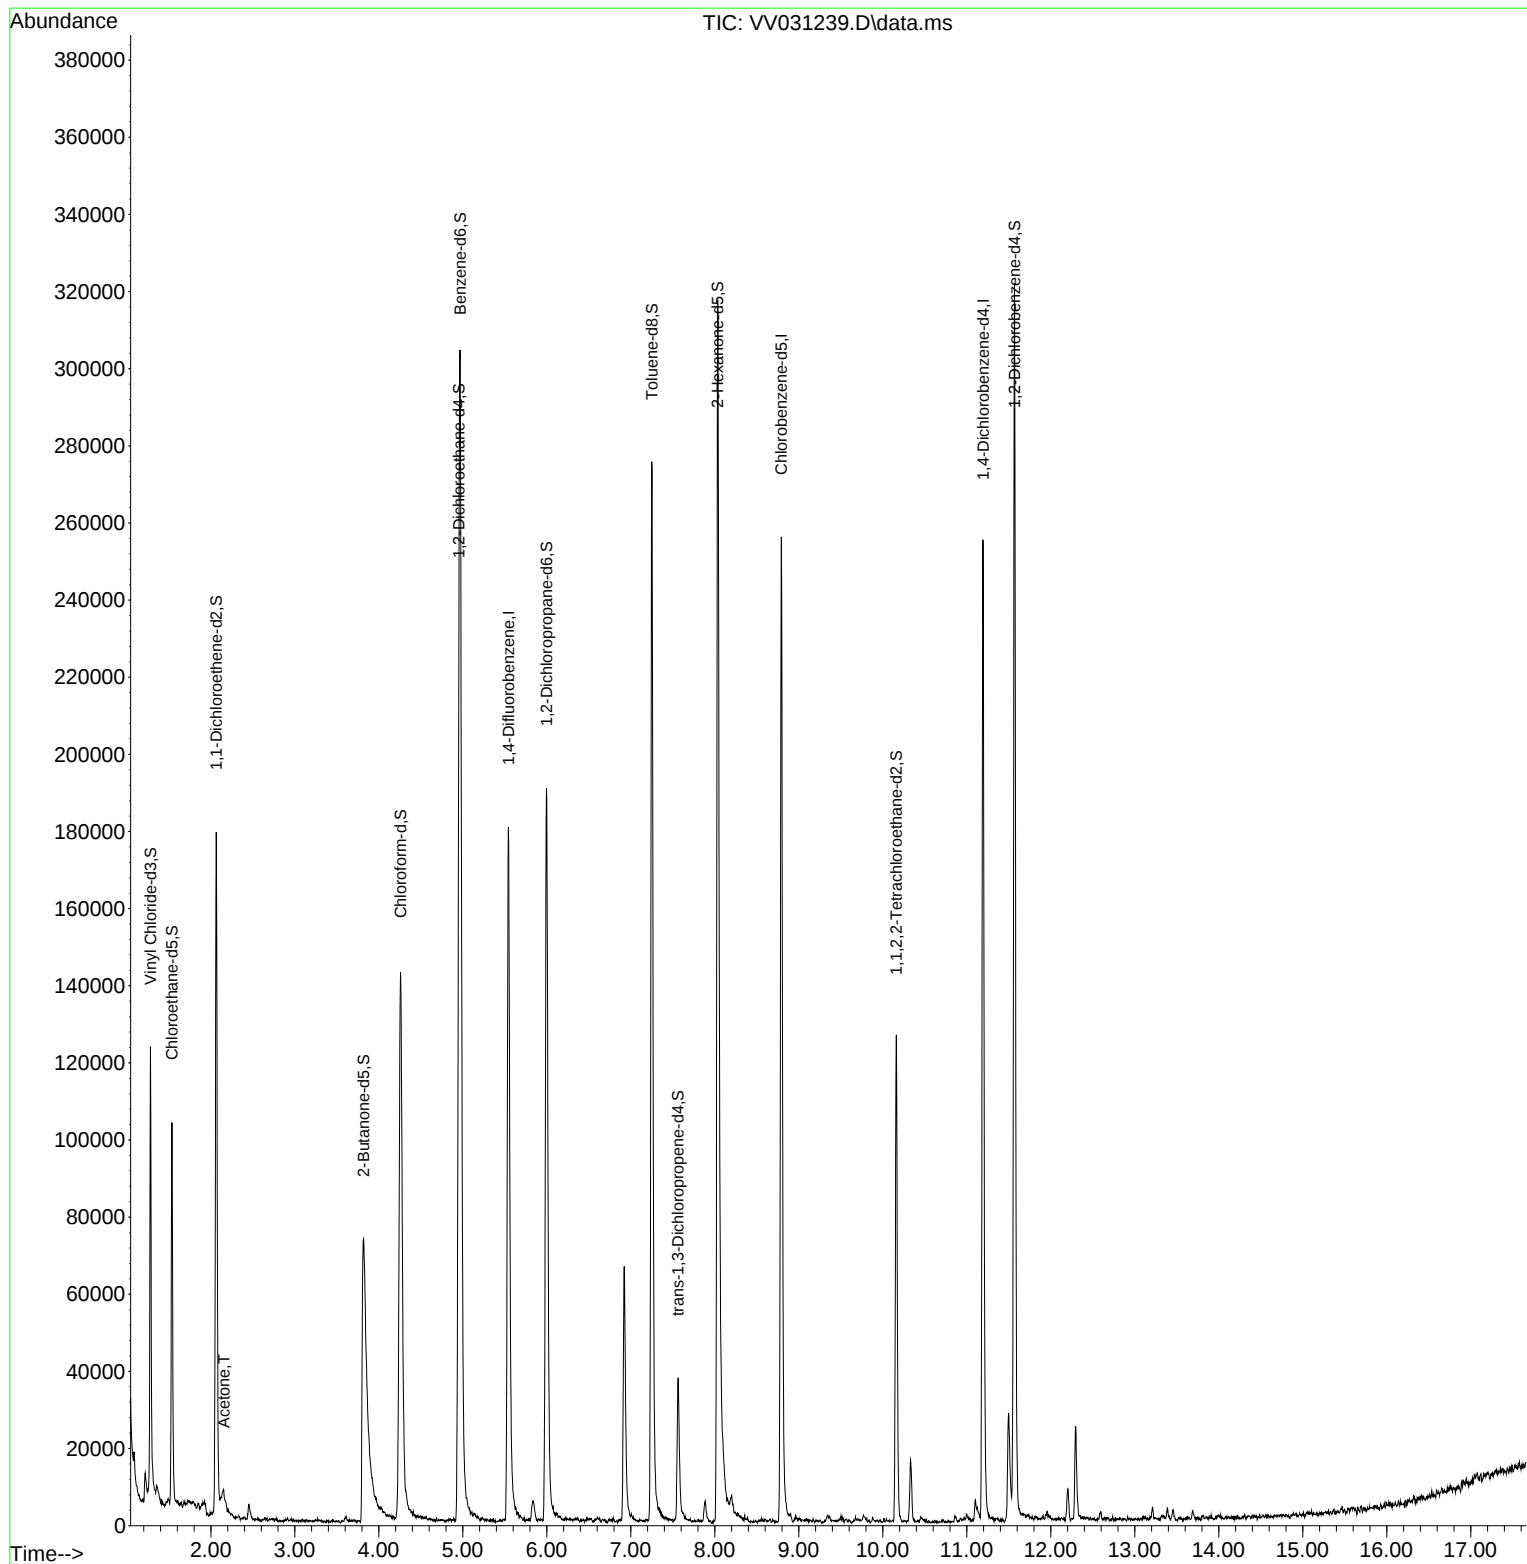

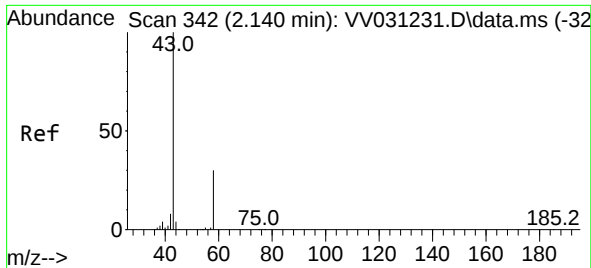

#13
Acetone
Concen: 4.749 ug/L m
RT: 2.153 min Scan# 34
Delta R.T. 0.013 min
Lab File: VV031239.D
Acq: 25 May 2023 17:59

Instrument :
MSVOA_V
ClientSampleId :
C11G5

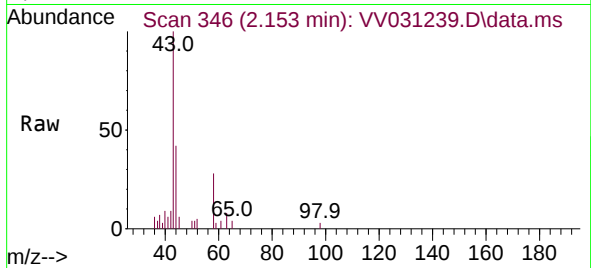

Tgt Ion: 43 Resp: 1289
Ion Ratio Lower Upper
43 100
58 17.5 0.0 62.2

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 05/26/2023
Supervised By :Mahesh Dadoda 05/26/2023

