

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052523\
 Data File : VV031240.D
 Acq On : 25 May 2023 18:23
 Operator : SY/MD
 Sample : 02917-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052523WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031240.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	90	rVB	118608	129083	15.76%	2.230%
2	1.539	146	155	169	rVB	100206	122183	14.92%	2.111%
3	2.063	306	318	334	rBV	167691	250408	30.57%	4.325%
4	3.822	852	865	907	rBV	74564	324794	39.65%	5.610%
5	4.259	984	1001	1026	rBV	144890	379679	46.35%	6.558%
6	4.966	1202	1221	1250	rBV2	312155	819106	100.00%	14.149%
7	5.542	1388	1400	1430	rBV	162451	348579	42.56%	6.021%
8	5.995	1527	1541	1562	rBV	174628	376787	46.00%	6.508%
9	6.921	1816	1829	1845	rBV	65800	127935	15.62%	2.210%
10	7.252	1919	1932	1951	rBV	293281	527755	64.43%	9.116%
11	7.561	2018	2028	2041	rBV3	42200	80770	9.86%	1.395%
12	7.886	2118	2129	2136	rBV2	6187	11063	1.35%	0.191%
13	8.037	2164	2176	2210	rBV	334271	717097	87.55%	12.387%
14	8.792	2399	2411	2435	rBV	251195	430460	52.55%	7.436%
15	10.159	2824	2836	2860	rBV	107908	180152	21.99%	3.112%
16	10.333	2877	2890	2901	rBV3	19084	31550	3.85%	0.545%
17	11.191	3146	3157	3181	rBV	255684	414492	50.60%	7.160%
18	11.567	3263	3274	3290	rVV	314229	504065	61.54%	8.707%
19	12.204	3462	3472	3484	rVB3	7926	13214	1.61%	0.228%




Sum of corrected areas: 5789172

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052523\
Data File : VV031240.D
Acq On : 25 May 2023 18:23
Operator : SY/MD
Sample : 02917-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052523WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

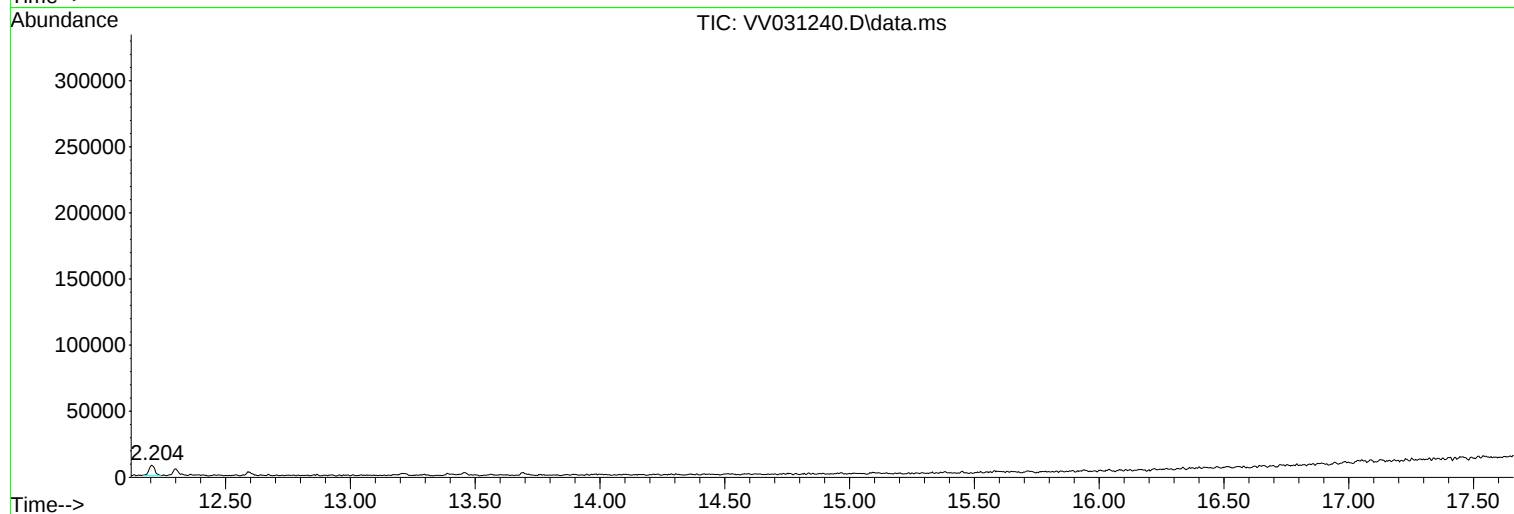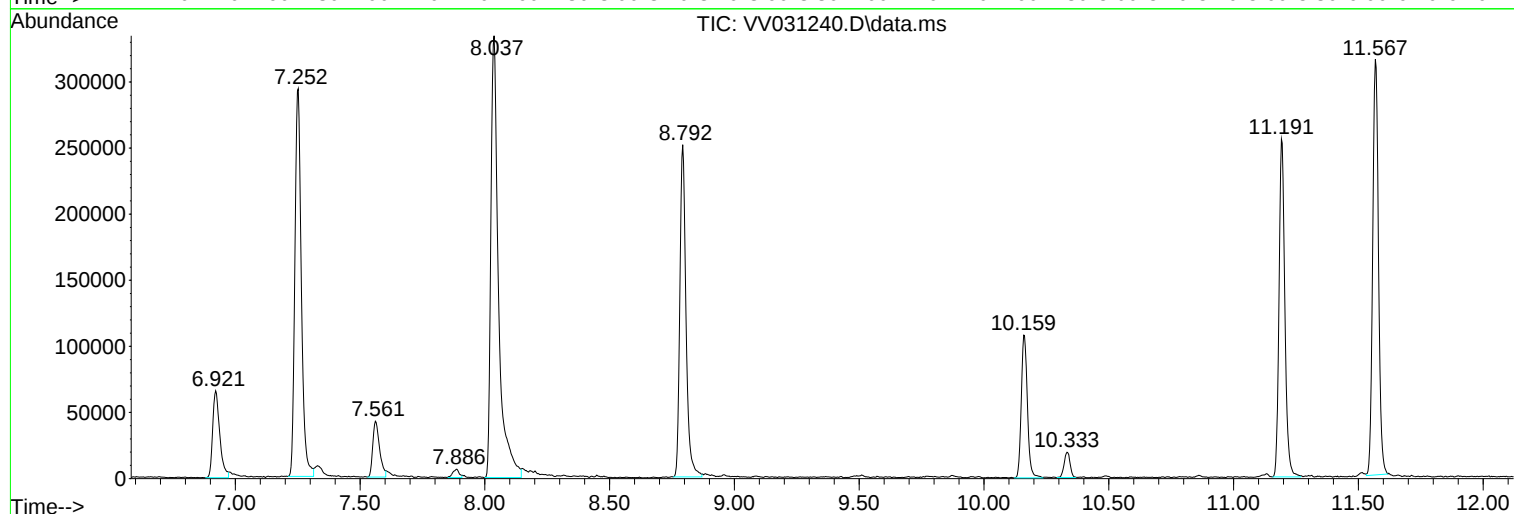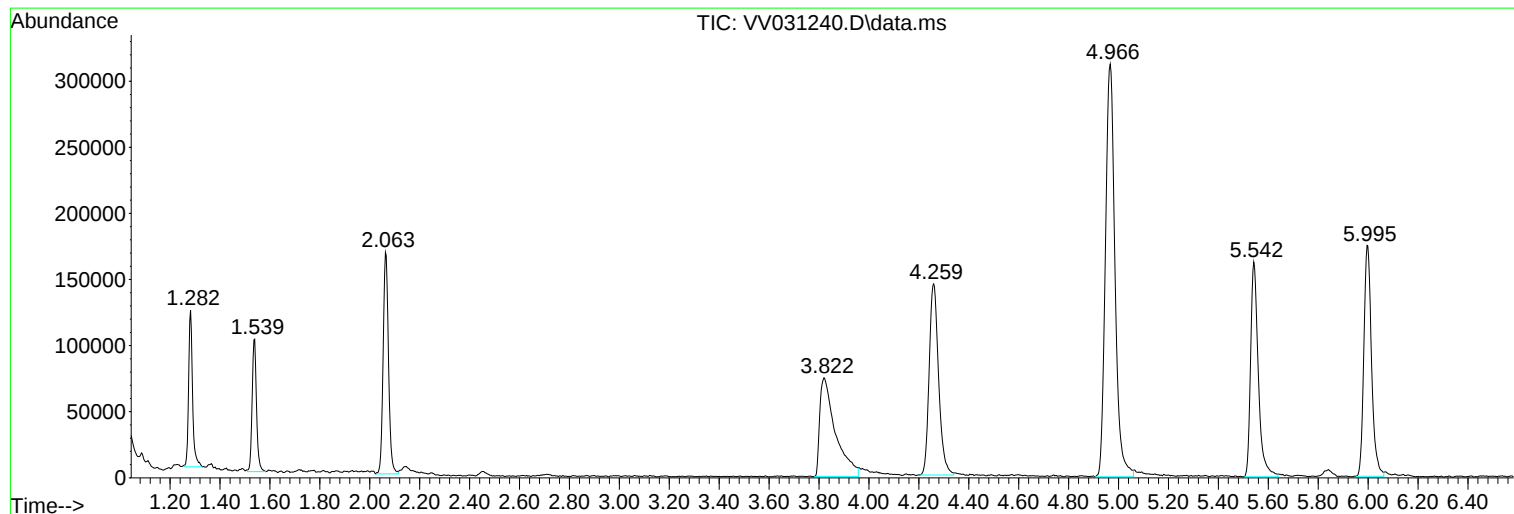

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW052523\
Data File : VW031240.D
Acq On : 25 May 2023 18:23
Operator : SY/MD
Sample : 02917-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052523WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052523\
Data File : VV031240.D
Acq On : 25 May 2023 18:23
Operator : SY/MD
Sample : 02917-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052523WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------