
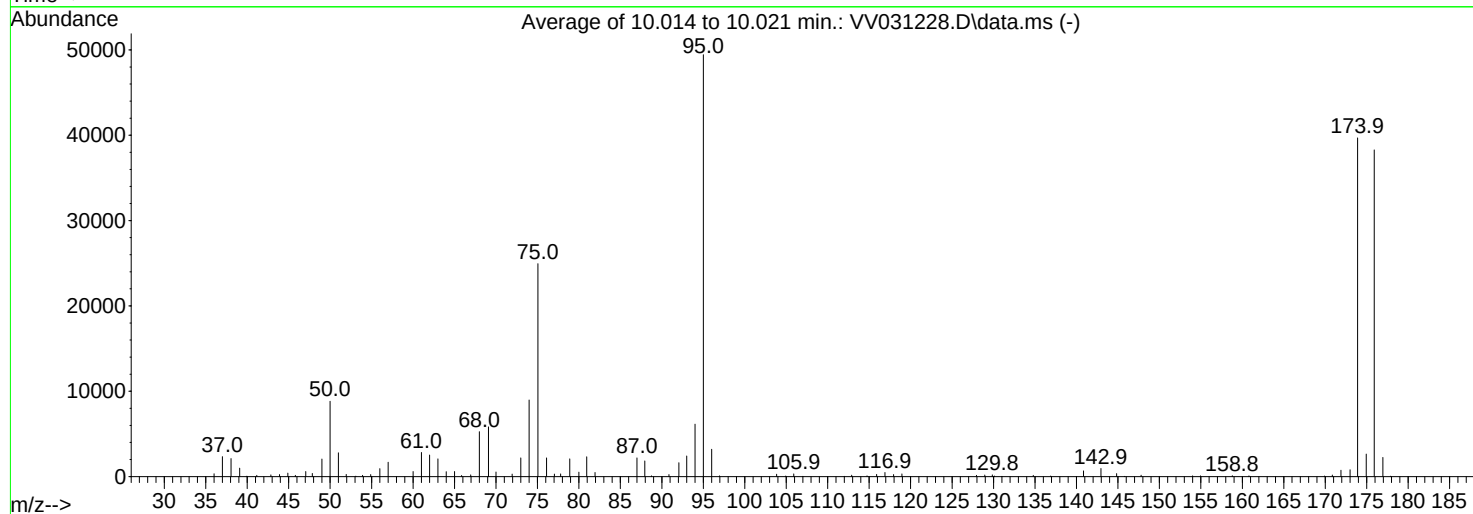


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052523\
 Data File : VV031228.D
 Acq On : 25 May 2023 10:04
 Operator : SY/MD
 Sample : BFB265
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB265

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052523WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri May 26 06:48:38 2023

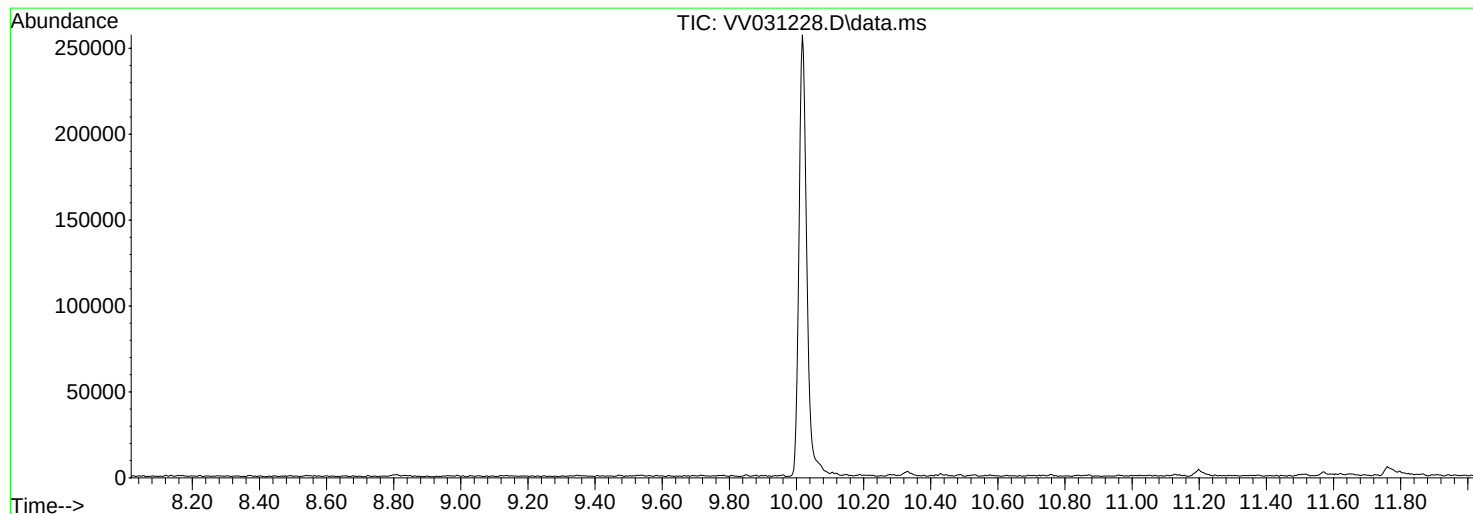

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	8818	PASS
75	95	30	80	50.5	24957	PASS
95	95	100	100	100.0	49435	PASS
96	95	5	9	6.5	3192	PASS
173	174	0.00	2	2.0	793	PASS
174	95	50	120	80.3	39685	PASS
175	174	5	9	6.7	2640	PASS
176	174	95	105	96.5	38291	PASS
177	176	5	10	5.9	2247	PASS

m/z	Abundance
36.10	138.0
39.90	268.0
44.00	409.0
45.00	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

m/z	Abundance
36.00	498.0
37.00	2273.0
38.10	1883.0
39.10	792.0
40.00	323.0
41.30	103.0
42.90	181.0
43.90	570.0
44.90	449.0
45.70	138.0
47.10	572.0
47.80	378.0
49.00	2048.0
50.00	8831.0
51.00	2924.0
52.00	224.0
53.90	131.0
54.90	151.0
56.00	945.0
57.00	1548.0
60.00	545.0
61.00	2761.0
62.00	2389.0
63.00	2209.0
64.00	529.0
65.00	528.0
65.80	122.0
67.00	207.0
68.00	5353.0
69.10	5896.0
70.00	537.0
72.00	347.0
73.00	2145.0
74.00	8678.0
75.00	24808.0
76.10	2253.0
77.00	269.0
77.80	201.0
78.90	2058.0
80.00	538.0
80.90	2126.0
81.90	543.0
87.00	2266.0
87.90	1831.0
88.70	137.0
90.80	284.0
92.10	1559.0
93.00	2279.0
94.00	5642.0
95.00	48096.0
96.00	3145.0
103.90	232.0
105.00	104.0
105.90	284.0
107.00	106.0
112.00	100.0
112.90	172.0
114.70	148.0
115.90	168.0
116.90	410.0
117.90	262.0
119.00	303.0
128.00	190.0
129.00	182.0
129.90	214.0
131.00	104.0
134.80	118.0
136.90	119.0
140.80	661.0
143.00	928.0
144.80	362.0
147.80	183.0
154.90	115.0
158.70	102.0
160.80	137.0
169.90	115.0
170.90	197.0
171.90	621.0
173.00	720.0
173.90	37664.0
175.00	2558.0
175.90	36088.0
177.00	2405.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

m/z	Abundance
36.00	479.0
37.00	2437.0
38.00	2247.0
39.10	1034.0
40.00	310.0
41.10	138.0
42.90	213.0
43.90	622.0
44.90	552.0
45.80	145.0
47.00	621.0
47.80	387.0
49.00	2120.0
50.00	9115.0
51.00	2882.0
51.90	290.0
53.90	160.0
54.90	243.0
56.00	946.0
57.00	1753.0
60.00	634.0
61.00	3005.0
62.00	2561.0
63.00	2095.0
64.00	561.0
65.00	623.0
65.80	128.0
67.00	212.0
68.00	5473.0
69.10	6086.0
70.00	569.0
71.90	264.0
73.00	2223.0
74.00	9213.0
75.10	25760.0
76.10	2245.0
77.10	293.0
77.80	325.0
78.90	2129.0
80.00	526.0
80.90	2376.0
82.00	501.0
87.00	2212.0
88.00	1822.0
88.80	106.0
90.90	258.0
92.00	1674.0
93.00	2541.0
94.00	6477.0
95.00	51328.0
96.00	3260.0
96.90	139.0
103.90	280.0
104.90	107.0
105.90	304.0
112.90	179.0
114.80	130.0
115.90	247.0
116.90	498.0
118.00	251.0
118.90	315.0
128.00	149.0
129.00	177.0
129.70	191.0
130.00	202.0
134.80	153.0
136.90	102.0
140.80	682.0
142.90	959.0
144.80	364.0
147.80	163.0
154.00	132.0
155.00	115.0
158.80	101.0
160.80	118.0
169.90	107.0
170.90	183.0
171.90	780.0
173.00	833.0
173.90	40984.0
175.00	2698.0
175.90	39688.0
176.90	2259.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

m/z	Abundance
36.00	414.0
37.00	2306.0
38.00	2203.0
39.10	1113.0
40.10	316.0
41.10	156.0
42.80	214.0
43.90	713.0
44.90	582.0
45.90	164.0
47.00	598.0
47.90	329.0
49.00	1969.0
50.00	8508.0
51.00	2569.0
51.90	248.0
53.10	122.0
53.90	162.0
54.90	288.0
56.00	870.0
57.00	1720.0
60.00	593.0
61.00	2697.0
62.00	2630.0
63.00	1903.0
64.00	604.0
65.00	640.0
65.90	116.0
66.90	175.0
68.00	4981.0
69.10	5468.0
70.00	511.0
71.90	257.0
73.00	2214.0
74.00	9034.0
75.10	24304.0
76.10	2077.0
77.00	303.0
77.80	397.0
78.90	2051.0
80.00	479.0
81.00	2455.0
82.00	407.0
87.00	2068.0
87.90	1822.0
90.80	188.0
92.00	1613.0
93.00	2419.0
94.00	6283.0
95.00	48880.0
96.00	3172.0
97.00	132.0
103.80	282.0
105.90	336.0
112.90	149.0
115.90	349.0
116.90	521.0
118.00	210.0
118.90	300.0
127.90	114.0
128.90	165.0
130.10	195.0
134.80	144.0
140.90	670.0
142.90	937.0
144.90	339.0
145.80	103.0
147.80	148.0
154.00	111.0
158.90	100.0
170.80	157.0
171.90	814.0
173.00	827.0
173.90	40408.0
174.90	2665.0
175.90	39096.0
176.90	2076.0
177.90	138.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265