

Data Path : W:\HPCHEM1\MSVOA V\DATA\VV052618\
 Data File : VV006076.D
 Acq On : 27 May 2018 01:21
 Operator : SY/MD
 Sample : J3092-15 100X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Quant Time: May 28 04:30:28 2018
 Quant Method : W:\HPCHEM1\MSVOA_V\METHOD\SOMVLM052518WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 28 02:03:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	164203	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	151027	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	60228	50.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.32	65	49422	43.10	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.20%
7) Chloroethane-d5	1.55	69	12364m	15.25	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	30.50%#
11) 1,1-Dichloroethene-d2	2.12	63	70350	32.96	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.92%
21) 2-Butanone-d5	3.95	46	53307	81.15	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	81.15%
24) Chloroform-d	4.40	84	98126	45.39	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.78%
26) 1,2-Dichloroethane-d4	5.09	65	68119	48.27	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.54%
32) Benzene-d6	5.10	84	193165	48.11	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.22%
36) 1,2-Dichloropropane-d6	6.12	67	62267	48.84	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.68%
41) Toluene-d8	7.36	98	164329	44.24	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.48%
43) trans-1,3-Dichloropropene-	7.67	79	24824	42.27	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.54%
47) 2-Hexanone-d5	8.14	63	50865	101.50	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	101.50%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	89048	50.79	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	101.58%
64) 1,2-Dichlorobenzene-d4	11.68	152	62505	52.18	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.36%


Target Compounds						Ovalue
34) Trichloroethene	5.96	95	58603	48.11	ug/L	99
46) Tetrachloroethene	8.02	164	3369	3.68	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA V\DATA\VV052618\
Data File : VV006076.D
Acq On : 27 May 2018 01:21
Operator : SY/MD
Sample : J3092-15 100X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 33 Sample Multiplier: 1

Quant Time: May 28 04:30:28 2018
Quant Method : W:\HPCHEM1\MSVOA_V\METHOD\SOMVLM052518WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 28 02:03:29 2018
Response via : Initial Calibration

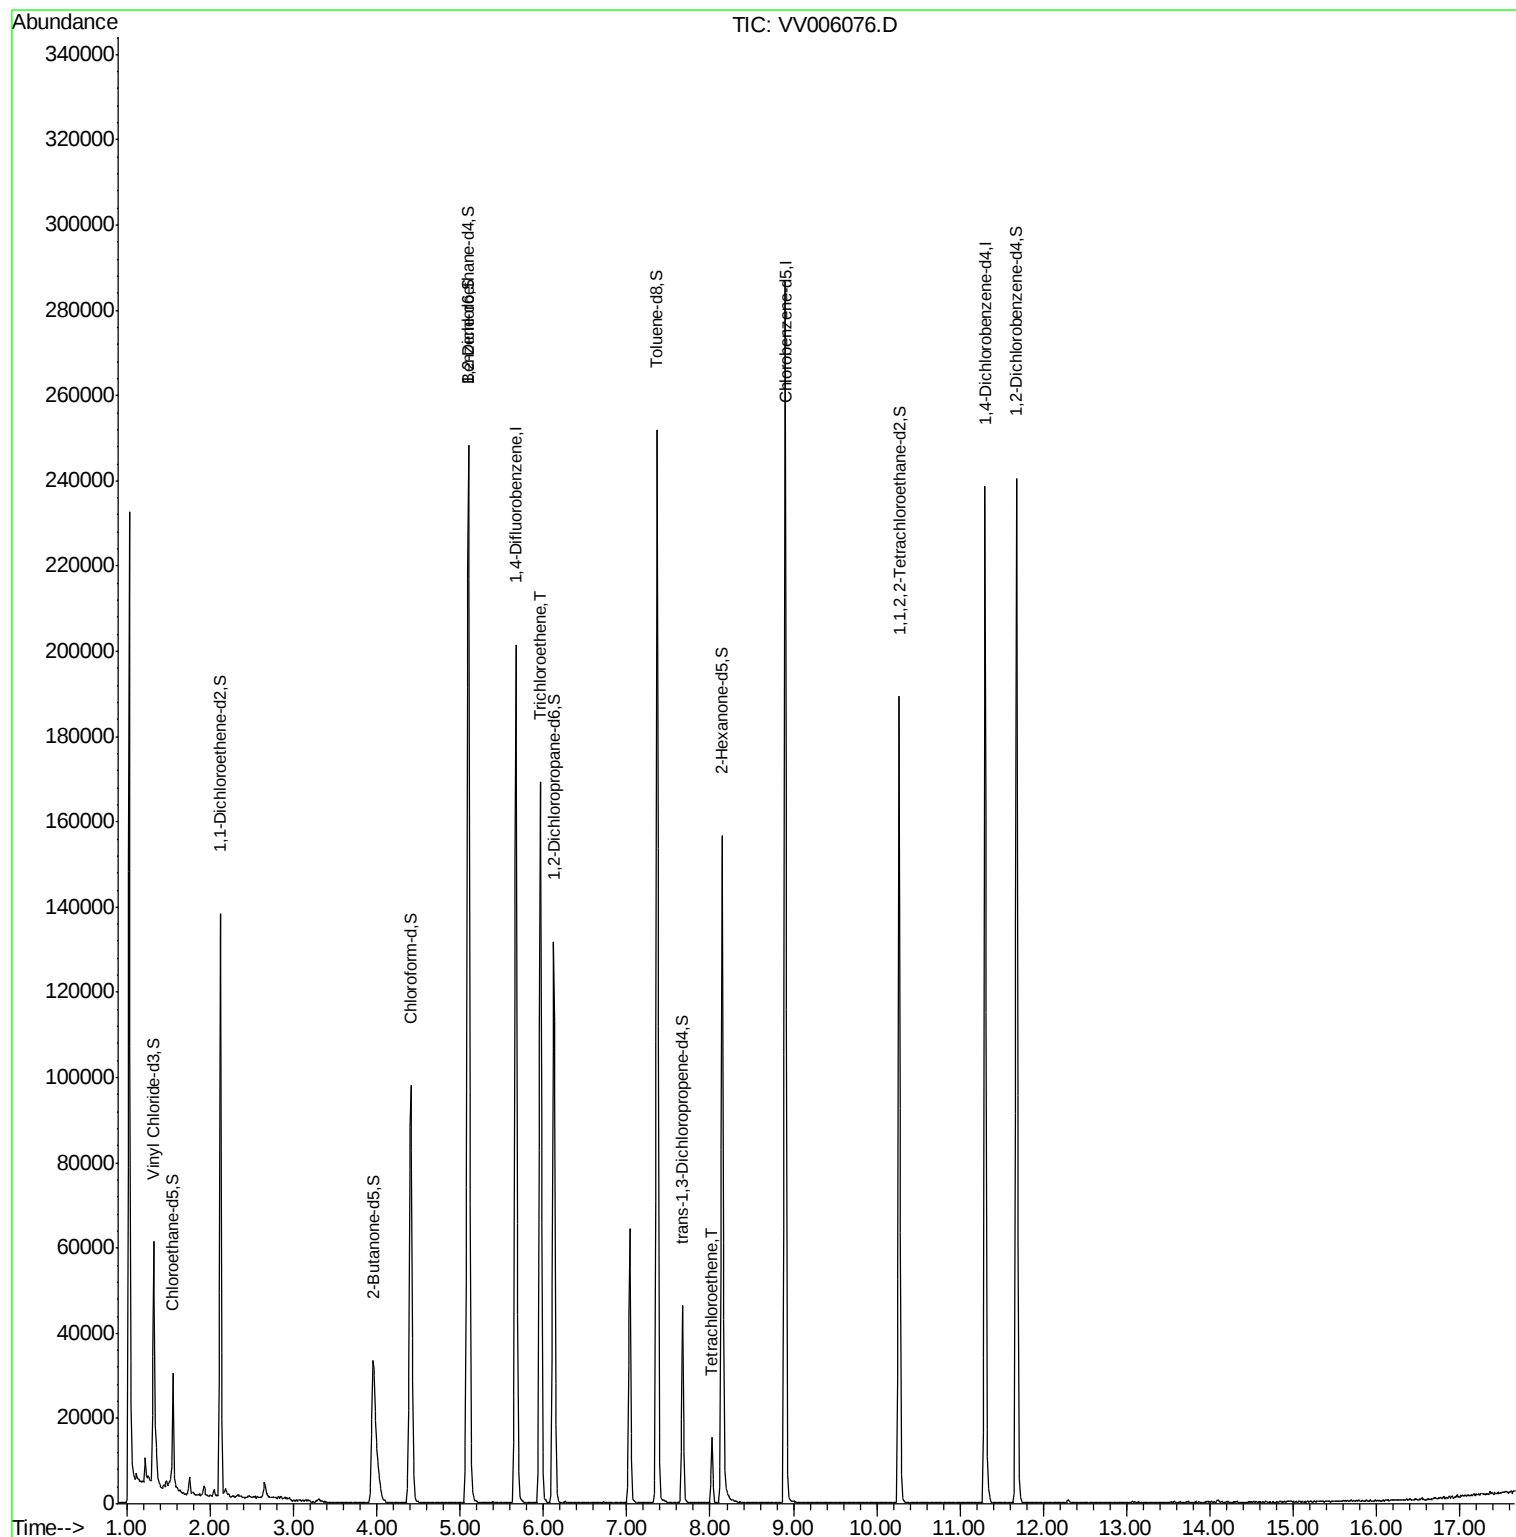

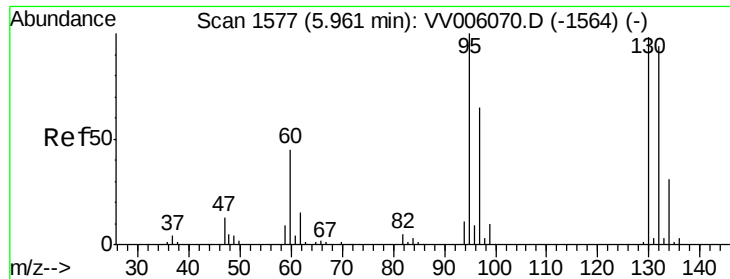

#34

Trichloroethene

Concen: 48.11 ug/L

RT: 5.96 min Scan# 1577

Delta R.T. 0.00 min

Lab File: VV006076.D

Acq: 27 May 2018 01:21

Tot Ion: 95 Resp: 58603


Ion Ratio Lower Upper

95 100

97 64.8 44.0 81.6

132 92.7 65.0 120.6

130 96.5 66.6 123.8



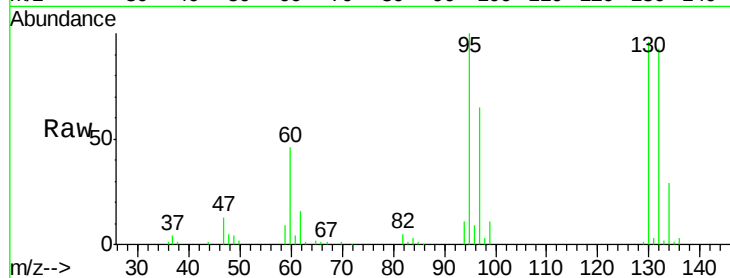


Abundance Ion 95.00 (94.70 to 95.70): VV0

Ion 97.00 (96.70 to 97.70): VV0

Ion 132.00 (131.70 to 132.70): V

Ion 130.00 (129.70 to 130.70): V

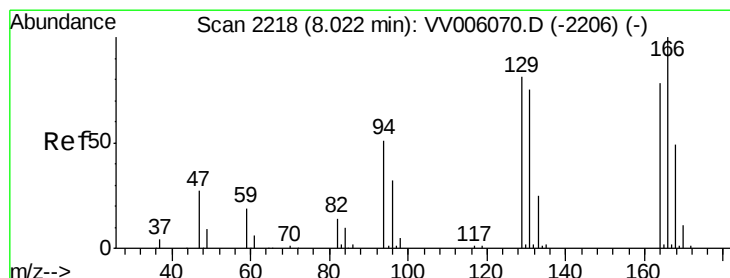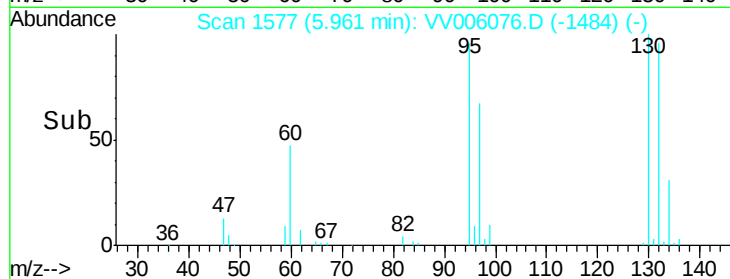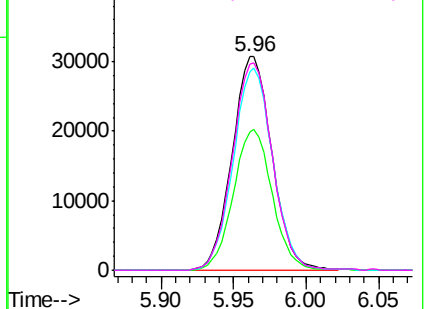

#46

Tetrachloroethene

Concen: 3.68 ug/L

RT: 8.02 min Scan# 2218

Delta R.T. 0.00 min

Lab File: VV006076.D

Acq: 27 May 2018 01:21

Tgt Ion: 164 Resp: 3369


Ion Ratio Lower Upper

164 100

129 97.9 72.2 134.2

131 96.5 70.0 130.0

166 123.7 90.4 167.8

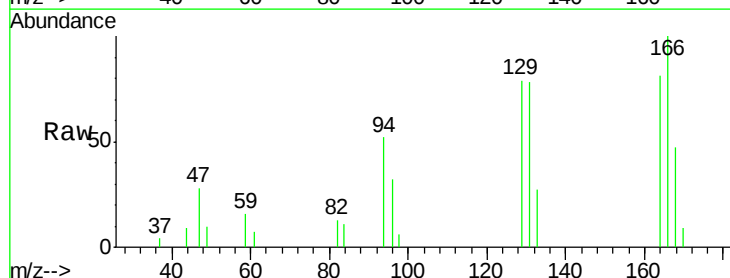

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

