


Data Path : W:\HPCHEM1\MSVOA V\DATA\VV052618\
Data File : VV006047.D
Acq On : 26 May 2018 10:11
Operator : SY/MD
Sample : BFB62
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : W:\HPCHEM1\MSVOA_V\METHOD\SOMVLM052518WMA.M
Title : VOC Analysis
Last Update : Mon May 28 02:03:29 2018

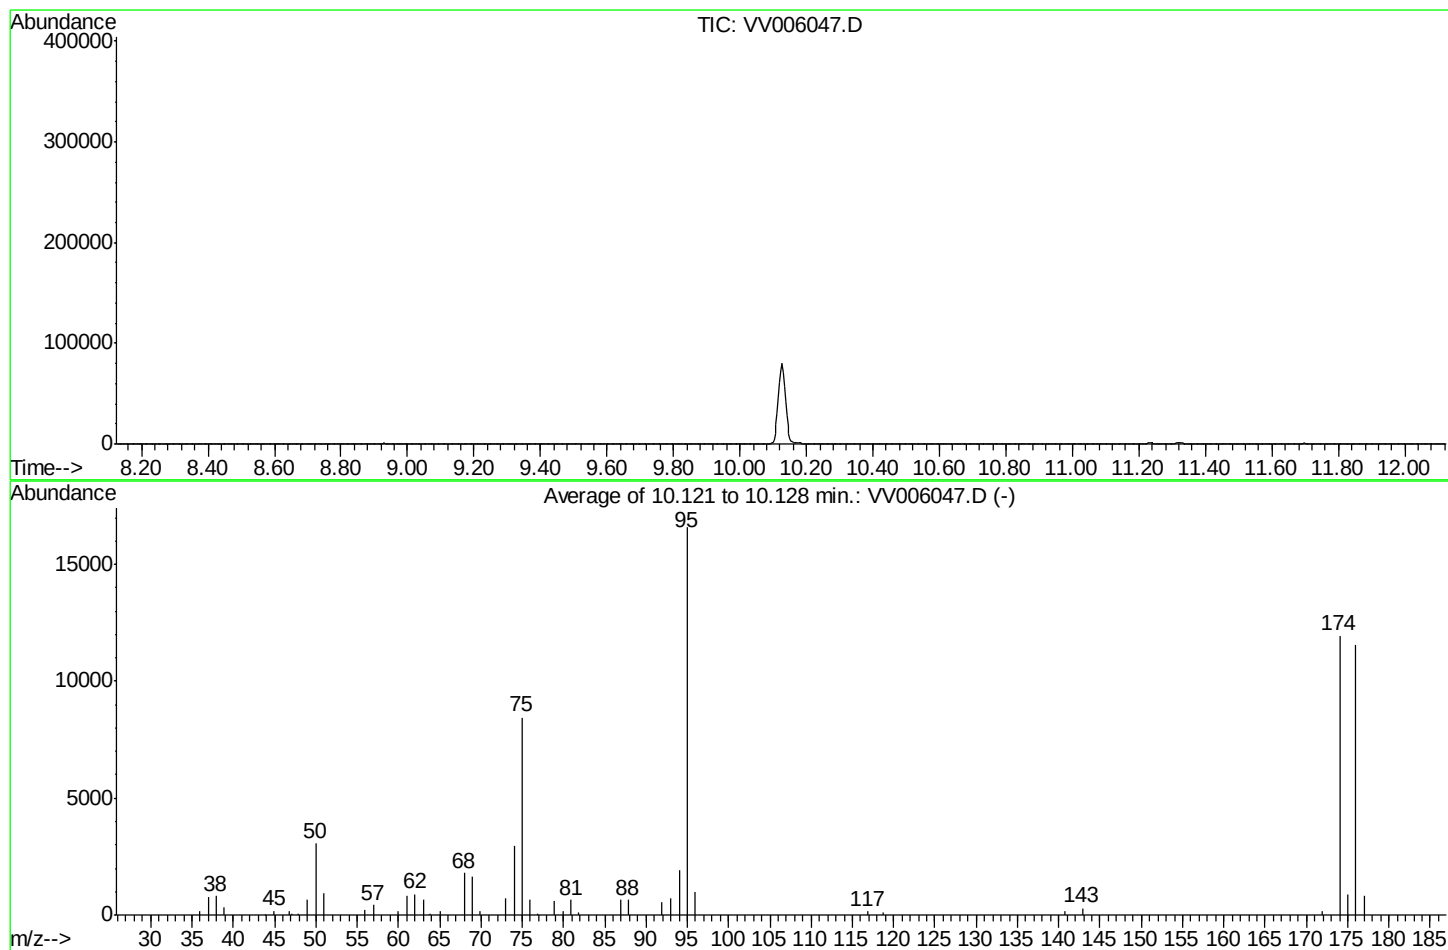

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2861

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	3057	PASS
75	95	30	80	50.9	8435	PASS
95	95	100	100	100.0	16582	PASS
96	95	5	9	6.1	1010	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.0	11941	PASS
175	174	5	9	7.3	876	PASS
176	174	95	101	96.6	11531	PASS
177	176	5	9	7.3	844	PASS