


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052620\  
Data File : VV016213.D  
Acq On : 27 May 2020 00:24  
Operator : SY/MD  
Sample : L2725-17  
Misc : 25.0mL/MSVOA V/WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
F9B34

Manual Integrations  
APPROVED

MMDadoda  
5/28/2020 5:16:43 PM

Quant Time: May 27 06:22:32 2020  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVTR052620WMA.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Wed May 27 03:06:56 2020  
Response via : Initial Calibration

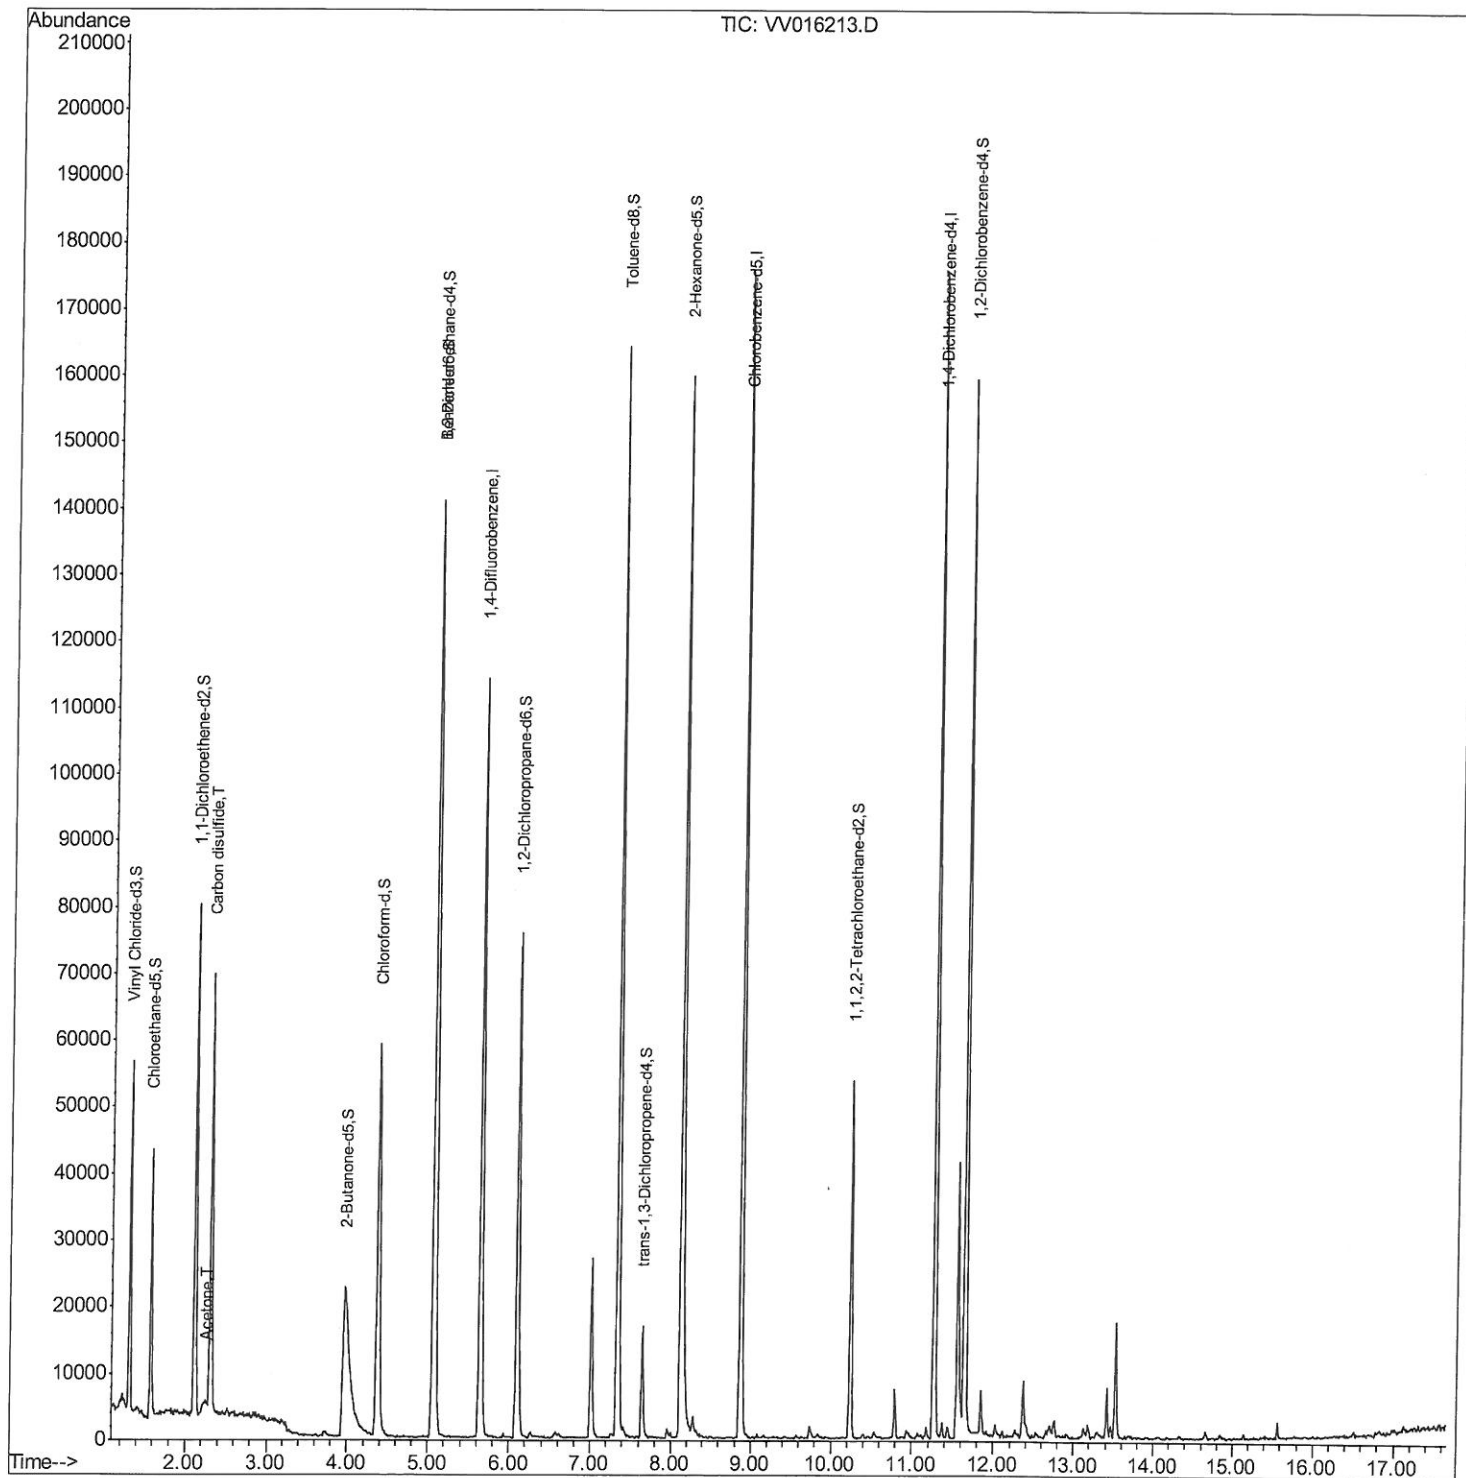


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052620\  
Data File : VV016213.D  
Acq On : 27 May 2020 00:24  
Operator : SY/MD  
Sample : L2725-17  
Misc : 25.0mL/MSVOA V/WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
F9B34

Manual Integrations  
APPROVED

MMDadoda  
5/28/2020 5:16:43 PM

Quant Time: May 27 03:18:52 2020  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVTR052620WMA.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Wed May 27 03:06:56 2020  
Response via : Initial Calibration

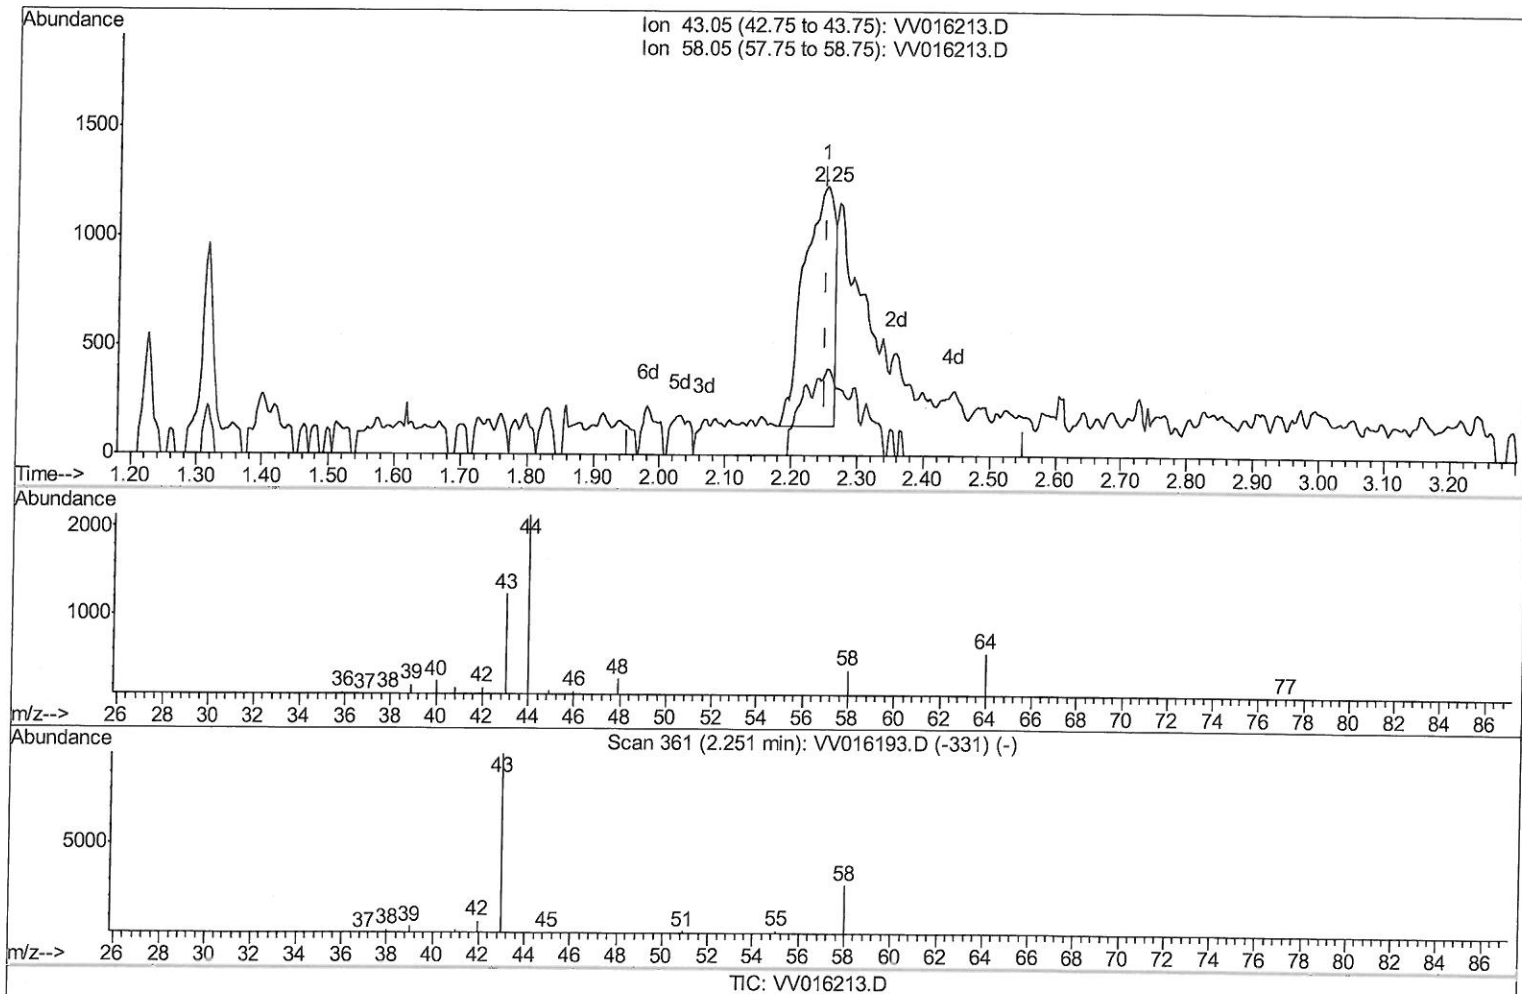

(13) Acetone (T)

2.251min (+0.000) 3.91ug/L

response 3478

| Ion   | Exp%  | Act%  |
|-------|-------|-------|
| 43.05 | 100   | 100   |
| 58.05 | 24.40 | 31.08 |
| 0.00  | 0.00  | 0.00  |
| 0.00  | 0.00  | 0.00  |

## Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052620\  
Data File : VV016213.D  
Acq On : 27 May 2020 00:24  
Operator : SY/MD  
Sample : L2725-17  
Misc : 25.0mL/MSVOA V/WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
F9B34

Manual Integrations  
APPROVED

MMDadoda  
5/28/2020 5:16:43 PM

Quant Time: Mav 27 03:18:52 2020  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVTR052620WMA.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Wed May 27 03:06:56 2020  
Response via : Initial Calibration

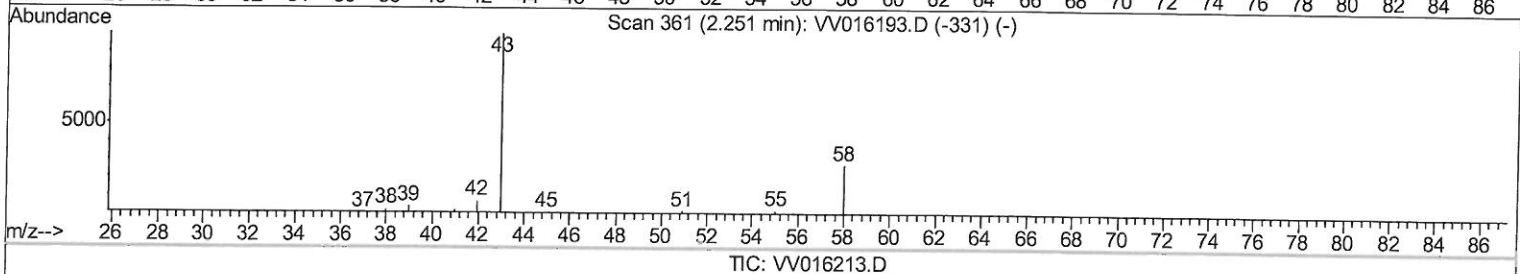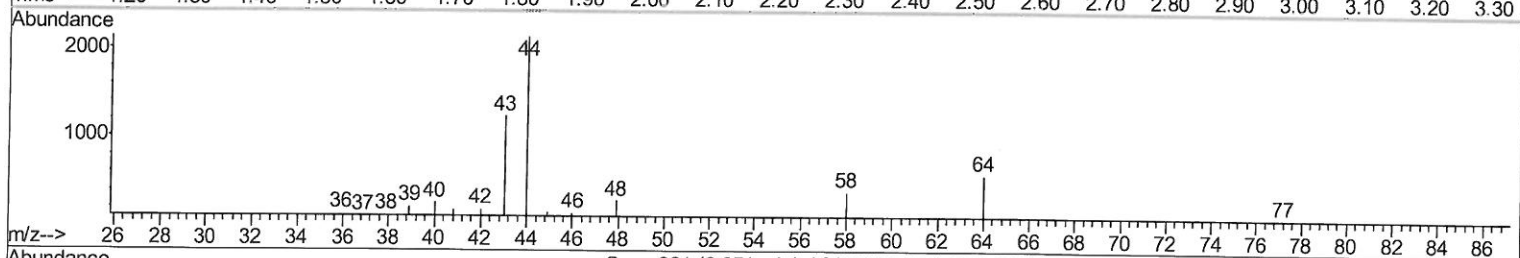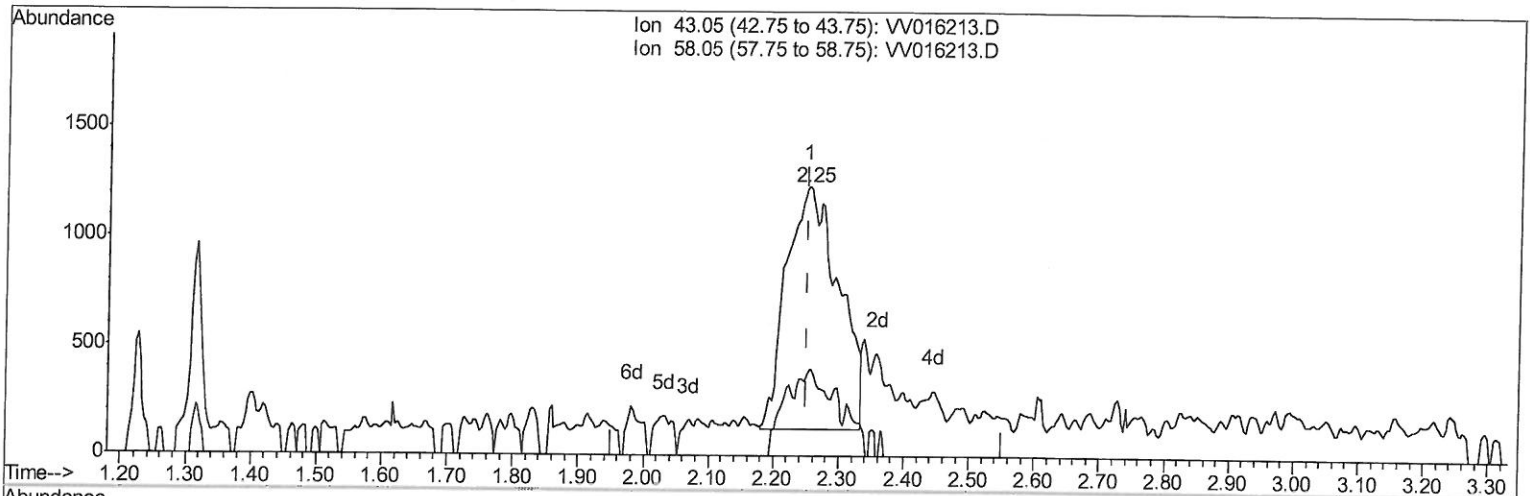

TIC: VV016213.D

(13) Acetone (T)

2.251min (+0.000) 6.93ug/L m

response 6173

| Ion   | Exp%  | Act%  |
|-------|-------|-------|
| 43.05 | 100   | 100   |
| 58.05 | 24.40 | 17.51 |
| 0.00  | 0.00  | 0.00  |
| 0.00  | 0.00  | 0.00  |

7 MB  
5/28/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052620\  
 Data File : VV016213.D  
 Acq On : 27 May 2020 00:24  
 Operator : SY/MD  
 Sample : L2725-17  
 Misc : 25.0mL/MSVOA V/WATER  
 ALS Vial : 25 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 F9B34

Manual Integrations  
 APPROVED

MMDadoda  
 5/28/2020 5:16:43 PM

Quant Time: May 27 06:22:32 2020  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVTR052620WMA.M  
 Quant Title : TRACE VOA SOM01.0  
 QLast Update : Wed May 27 03:06:56 2020  
 Response via : Initial Calibration

| Internal Standards             | R.T.           | QIon | Response           | Conc  | Units | Dev(Min) |
|--------------------------------|----------------|------|--------------------|-------|-------|----------|
| 1) 1,4-Difluorobenzene         | 5.64           | 114  | 90271              | 5.00  | ug/L  | 0.00     |
| 28) Chlorobenzene-d5           | 8.87           | 117  | 88634              | 5.00  | ug/L  | 0.00     |
| 61) 1,4-Dichlorobenzene-d4     | 11.27          | 152  | 40187              | 5.00  | ug/L  | 0.00     |
| System Monitoring Compounds    |                |      |                    |       |       |          |
| 4) Vinyl Chloride-d3           | 1.32           | 65   | 30322              | 5.23  | ug/L  | 0.00     |
| Spiked Amount 5.000            | Range 40 - 130 |      | Recovery = 104.60% |       |       |          |
| 7) Chloroethane-d5             | 1.58           | 69   | 26115              | 5.13  | ug/L  | 0.00     |
| Spiked Amount 5.000            | Range 65 - 130 |      | Recovery = 102.60% |       |       |          |
| 11) 1,1-Dichloroethene-d2      | 2.12           | 63   | 41057              | 3.77  | ug/L  | 0.00     |
| Spiked Amount 5.000            | Range 60 - 125 |      | Recovery = 75.40%  |       |       |          |
| 20) 2-Butanone-d5              | 3.97           | 46   | 76512              | 53.20 | ug/L  | 0.00     |
| Spiked Amount 50.000           | Range 40 - 130 |      | Recovery = 106.40% |       |       |          |
| 24) Chloroform-d               | 4.38           | 84   | 58846              | 5.10  | ug/L  | 0.00     |
| Spiked Amount 5.000            | Range 70 - 125 |      | Recovery = 102.00% |       |       |          |
| 26) 1,2-Dichloroethane-d4      | 5.06           | 65   | 32346              | 5.29  | ug/L  | 0.00     |
| Spiked Amount 5.000            | Range 70 - 130 |      | Recovery = 105.80% |       |       |          |
| 32) Benzene-d6                 | 5.07           | 84   | 115502             | 5.26  | ug/L  | 0.00     |
| Spiked Amount 5.000            | Range 70 - 125 |      | Recovery = 105.20% |       |       |          |
| 36) 1,2-Dichloropropane-d6     | 6.10           | 67   | 35203              | 5.18  | ug/L  | 0.00     |
| Spiked Amount 5.000            | Range 60 - 140 |      | Recovery = 103.60% |       |       |          |
| 41) Toluene-d8                 | 7.34           | 98   | 102539             | 4.90  | ug/L  | 0.00     |
| Spiked Amount 5.000            | Range 70 - 130 |      | Recovery = 98.00%  |       |       |          |
| 45) trans-1,3-Dichloropropene- | 7.65           | 79   | 9656               | 3.81  | ug/L  | 0.00     |
| Spiked Amount 5.000            | Range 55 - 130 |      | Recovery = 76.20%  |       |       |          |
| 48) 2-Hexanone-d5              | 8.12           | 63   | 52721              | 45.40 | ug/L  | 0.00     |
| Spiked Amount 50.000           | Range 45 - 130 |      | Recovery = 90.80%  |       |       |          |
| 59) 1,1,2,2-Tetrachloroethane- | 10.24          | 84   | 24977              | 4.98  | ug/L  | 0.00     |
| Spiked Amount 5.000            | Range 65 - 120 |      | Recovery = 99.60%  |       |       |          |
| 65) 1,2-Dichlorobenzene-d4     | 11.65          | 152  | 36236              | 5.40  | ug/L  | 0.00     |
| Spiked Amount 5.000            | Range 80 - 120 |      | Recovery = 108.00% |       |       |          |
| Target Compounds               |                |      |                    |       |       |          |
| 13) Acetone                    | 2.25           | 43   | 6173m              | 6.934 | ug/L  | Ovalue   |
| 14) Carbon disulfide           | 2.31           | 76   | 70574              | 4.276 | ug/L  | 99       |

(#) = qualifier out of range (m) = manual integration (+) = signals summed