

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052620\
 Data File : VV016202.D
 Acq On : 26 May 2020 19:57
 Operator : SY/MD
 Sample : L2731-13
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX8

Quant Time: May 27 05:15:55 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR052620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed May 27 03:06:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	100792	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	96559	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	44906	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	29392	4.54	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.80%
7) Chloroethane-d5	1.58	69	26706	4.70	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.00%
11) 1,1-Dichloroethene-d2	2.12	63	41285	3.40	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.00%
20) 2-Butanone-d5	3.96	46	83630	52.08	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.16%
24) Chloroform-d	4.38	84	60899	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
26) 1,2-Dichloroethane-d4	5.06	65	33409	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.00%
32) Benzene-d6	5.08	84	120779	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.00%
36) 1,2-Dichloropropane-d6	6.10	67	37732	5.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.00%
41) Toluene-d8	7.34	98	110069	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
45) trans-1,3-Dichloropropene-	7.65	79	12922	4.68	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.60%
48) 2-Hexanone-d5	8.12	63	62927	49.74	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.48%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	25559	4.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.40%
65) 1,2-Dichlorobenzene-d4	11.65	152	38685	5.16	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.20%


Target Compounds					Ovalue
9) Trichlorofluoromethane	1.77	101	2109	0.185 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052620\
Data File : VV016202.D
Acq On : 26 May 2020 19:57
Operator : SY/MD
Sample : L2731-13
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX8

Quant Time: May 27 05:15:55 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR052620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed May 27 03:06:56 2020
Response via : Initial Calibration

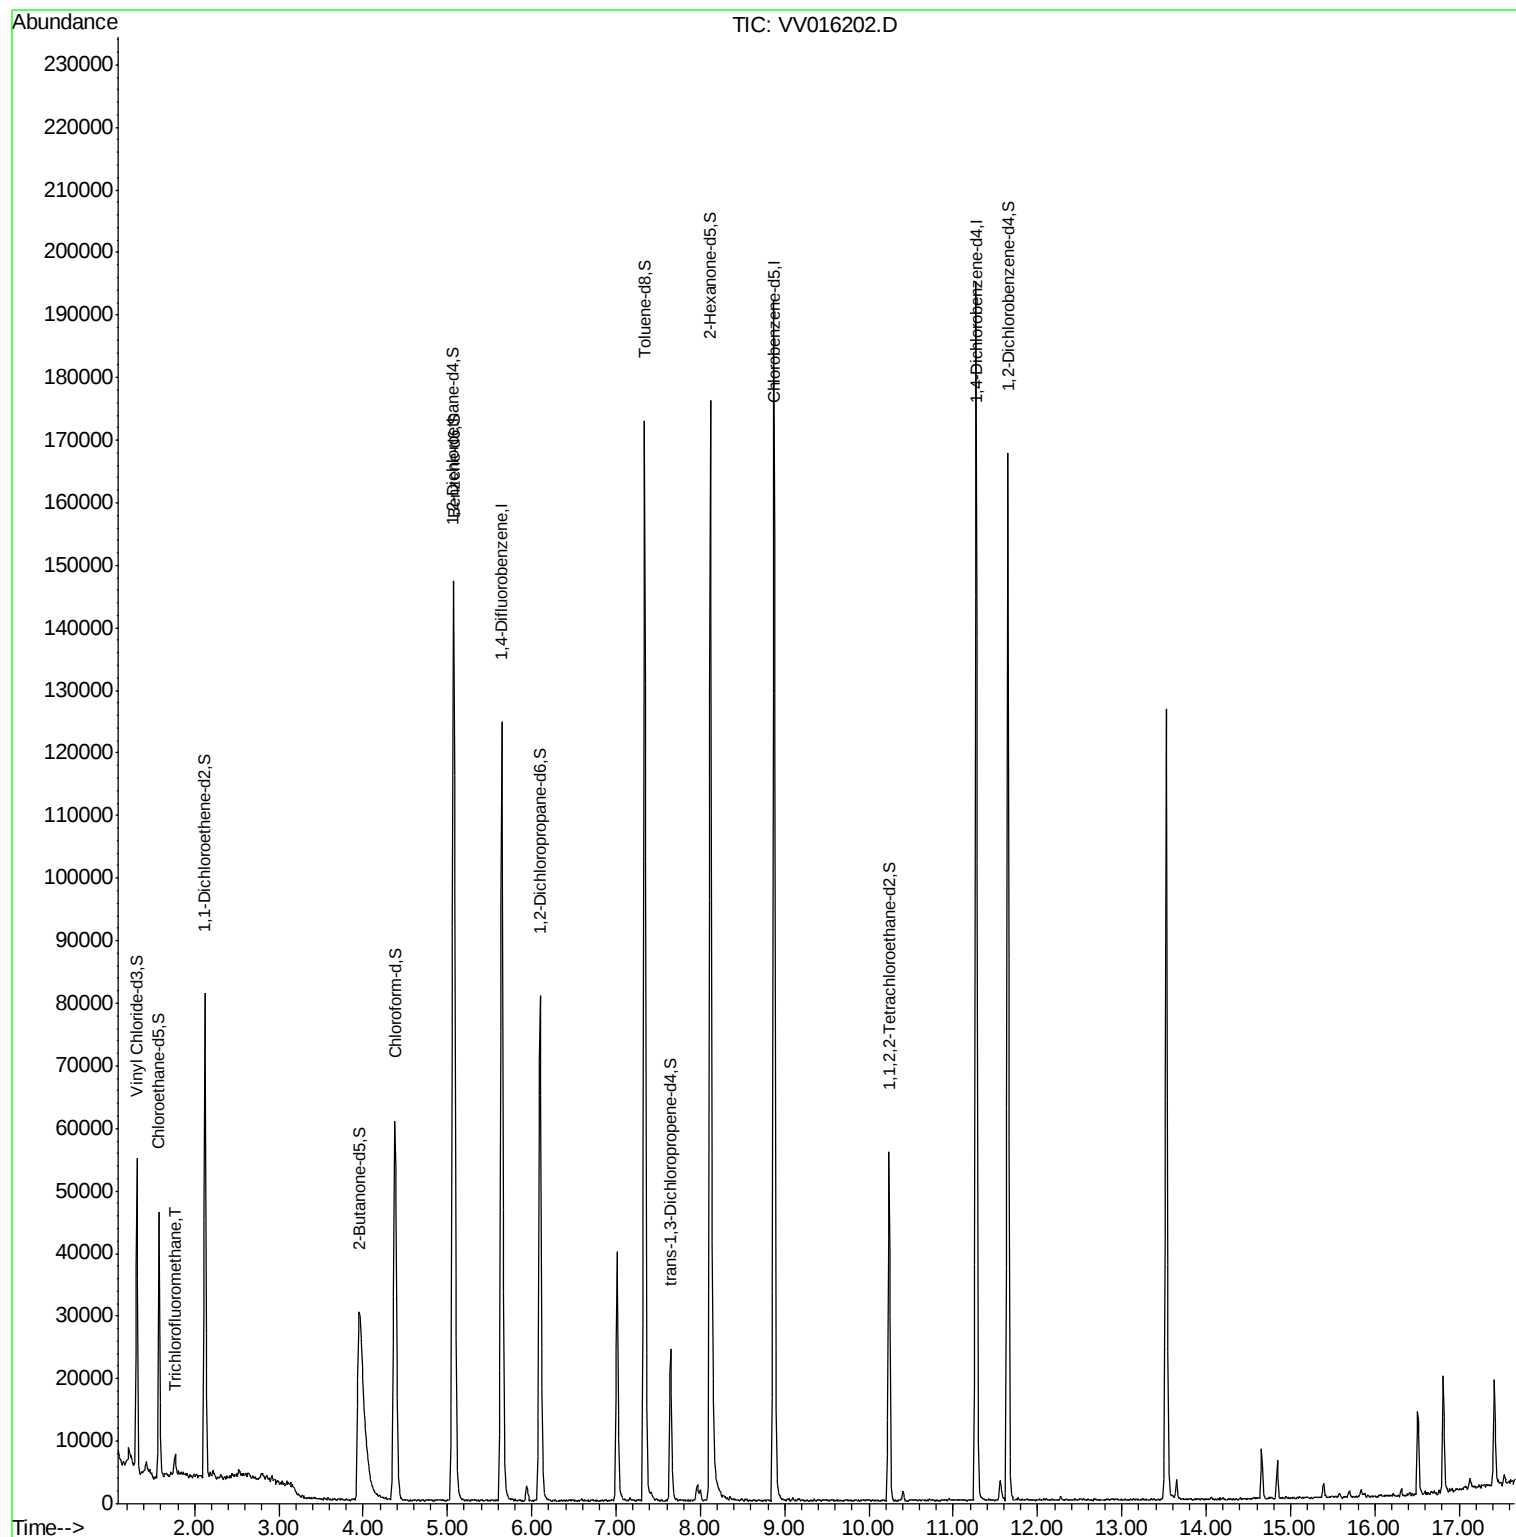

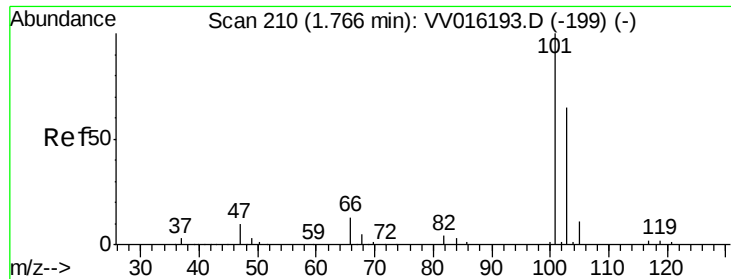

#9
 Trichlorofluoromethane
 Concen: 0.185 ug/L
 RT: 1.77 min Scan# 210
 Delta R.T. 0.00 min
 Lab File: VV016202.D
 Acq: 26 May 2020 19:57

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX8

Tot Ion:101 Resp: 2109
 Ion Ratio Lower Upper
 101 100
 103 60.2 51.9 77.9

