

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052620\
 Data File : VV016203.D
 Acq On : 26 May 2020 20:22
 Operator : SY/MD
 Sample : L2731-12
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX7

Quant Time: May 27 05:19:59 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR052620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed May 27 03:06:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	97728	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	94194	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	44158	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	29971	4.77	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.40%
7) Chloroethane-d5	1.58	69	26289	4.77	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.40%
11) 1,1-Dichloroethene-d2	2.13	63	41161	3.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.80%
20) 2-Butanone-d5	3.95	46	80622	51.78	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.56%
24) Chloroform-d	4.38	84	60430	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
26) 1,2-Dichloroethane-d4	5.06	65	32689	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.80%
32) Benzene-d6	5.08	84	117820	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.00%
36) 1,2-Dichloropropane-d6	6.10	67	36893	5.11	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.20%
41) Toluene-d8	7.34	98	108122	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.20%
45) trans-1,3-Dichloropropene-	7.65	79	12490	4.64	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.80%
48) 2-Hexanone-d5	8.12	63	59512	48.22	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.44%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	25599	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.00%
65) 1,2-Dichlorobenzene-d4	11.65	152	37287	5.06	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.20%


Target Compounds					Ovalue
9) Trichlorofluoromethane	1.77	101	1635	0.148 ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052620\
Data File : VV016203.D
Acq On : 26 May 2020 20:22
Operator : SY/MD
Sample : L2731-12
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX7

Quant Time: May 27 05:19:59 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR052620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed May 27 03:06:56 2020
Response via : Initial Calibration

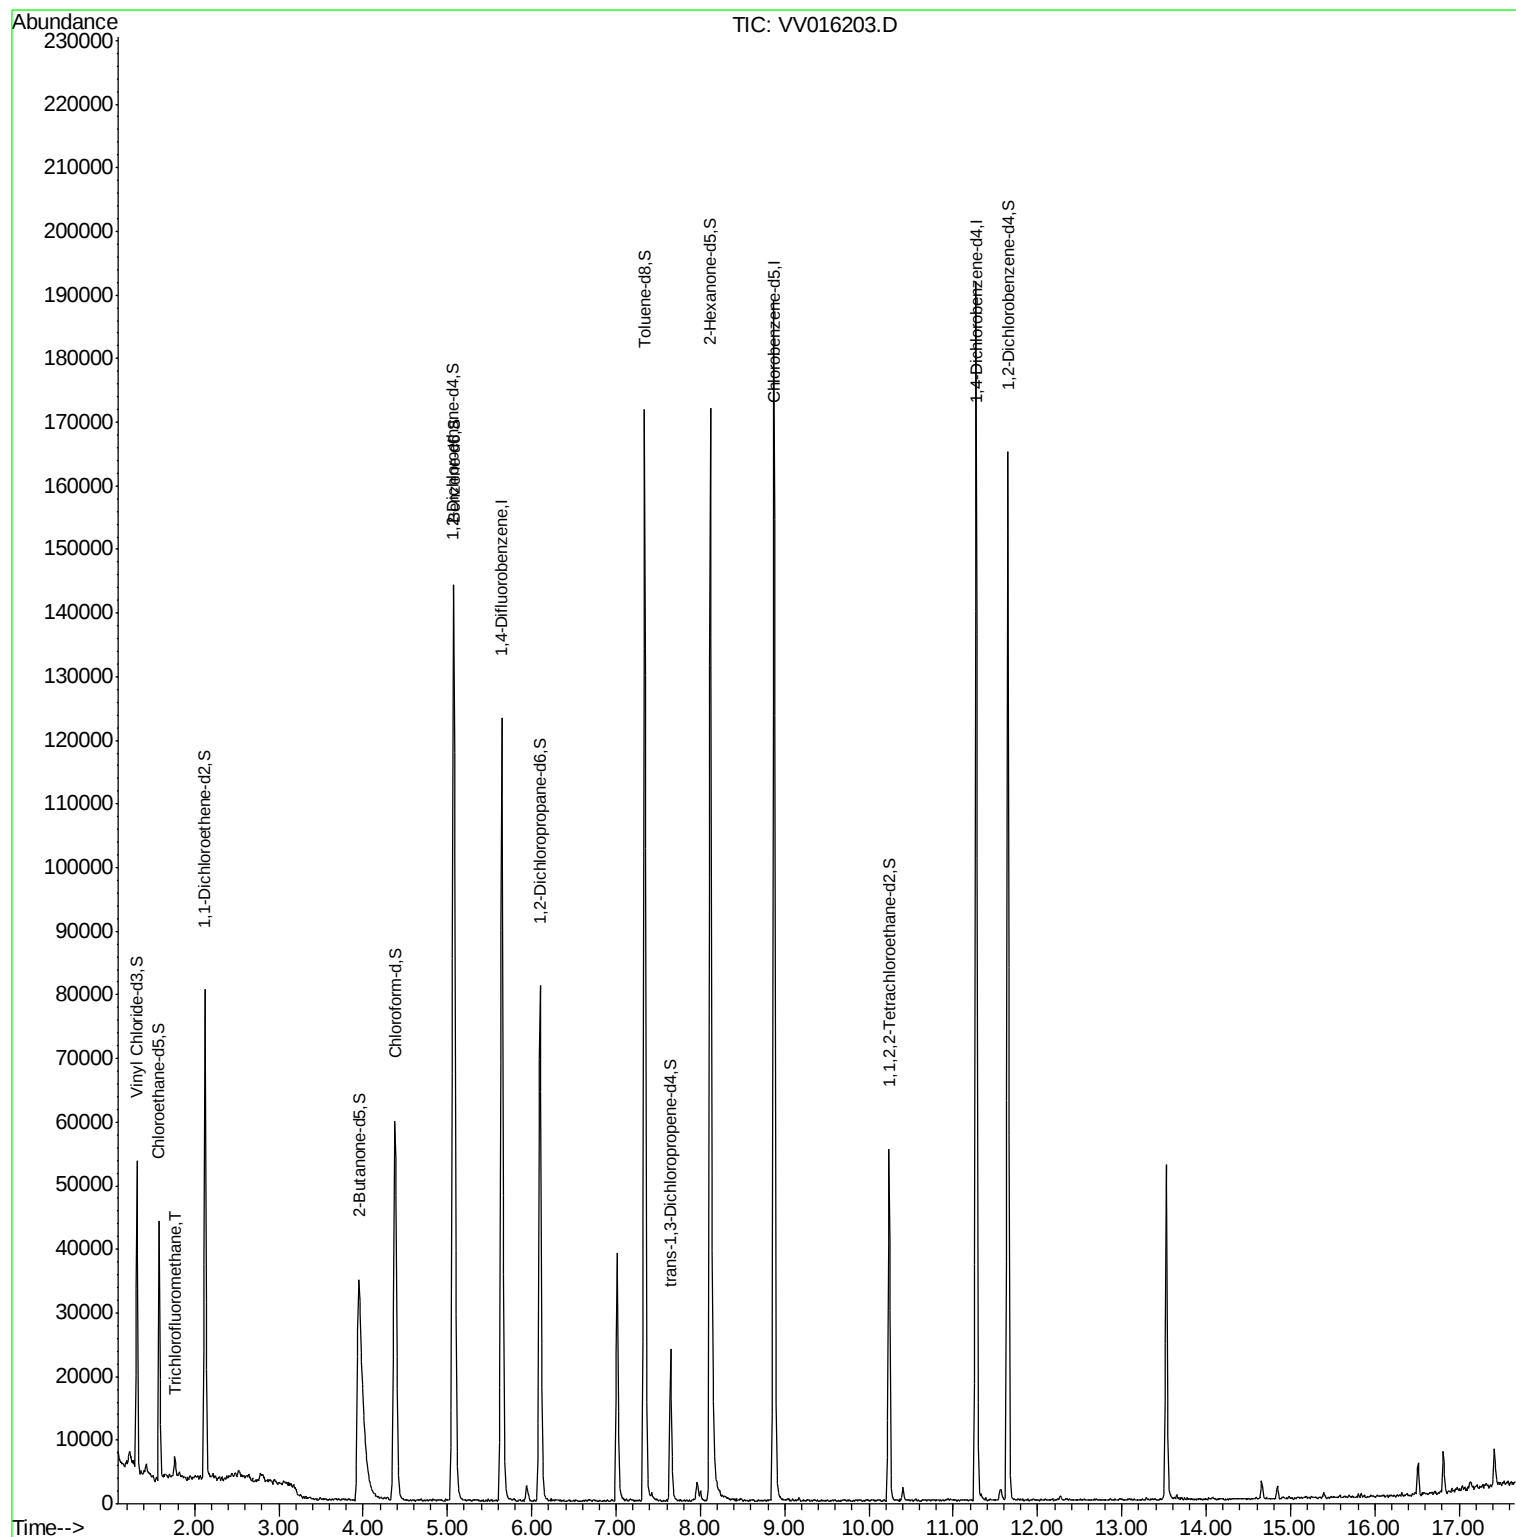

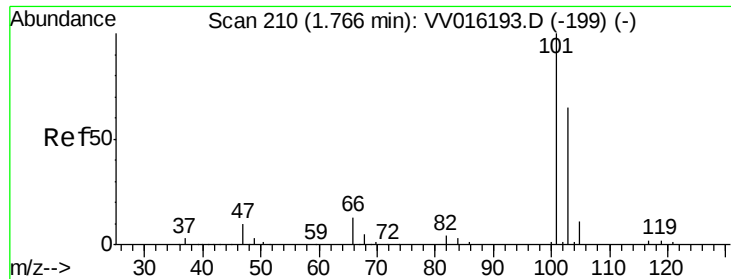

#9

Trichlorofluoromethane
 Concen: 0.148 ug/L
 RT: 1.77 min Scan# 211
 Delta R.T. 0.00 min
 Lab File: VV016203.D
 Acq: 26 May 2020 20:22

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX7

Tot Ion:101 Resp: 1635
 Ion Ratio Lower Upper
 101 100
 103 76.3 51.9 77.9

