

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052620\
 Data File : VV016211.D
 Acq On : 26 May 2020 23:35
 Operator : SY/MD
 Sample : L2753-20
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAXF7

Quant Time: May 27 06:14:14 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR052620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed May 27 03:06:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.65	114	93531	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	89380	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	41299	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	29026	4.83	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.60%
7) Chloroethane-d5	1.58	69	26269	4.98	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.60%
11) 1,1-Dichloroethene-d2	2.13	63	40578	3.60	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.00%
20) 2-Butanone-d5	3.93	46	76884	51.60	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.20%
24) Chloroform-d	4.38	84	57249	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
26) 1,2-Dichloroethane-d4	5.06	65	30795	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.20%
32) Benzene-d6	5.08	84	112552	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.60%
36) 1,2-Dichloropropane-d6	6.10	67	34170	4.99	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.80%
41) Toluene-d8	7.34	98	101242	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.00%
45) trans-1,3-Dichloropropene-	7.65	79	12073	4.73	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.60%
48) 2-Hexanone-d5	8.12	63	53807	45.95	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.90%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	24170	4.77	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.40%
65) 1,2-Dichlorobenzene-d4	11.65	152	35677	5.17	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	3603	3.906 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052620\
Data File : VV016211.D
Acq On : 26 May 2020 23:35
Operator : SY/MD
Sample : L2753-20
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAXF7

Quant Time: May 27 06:14:14 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR052620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed May 27 03:06:56 2020
Response via : Initial Calibration

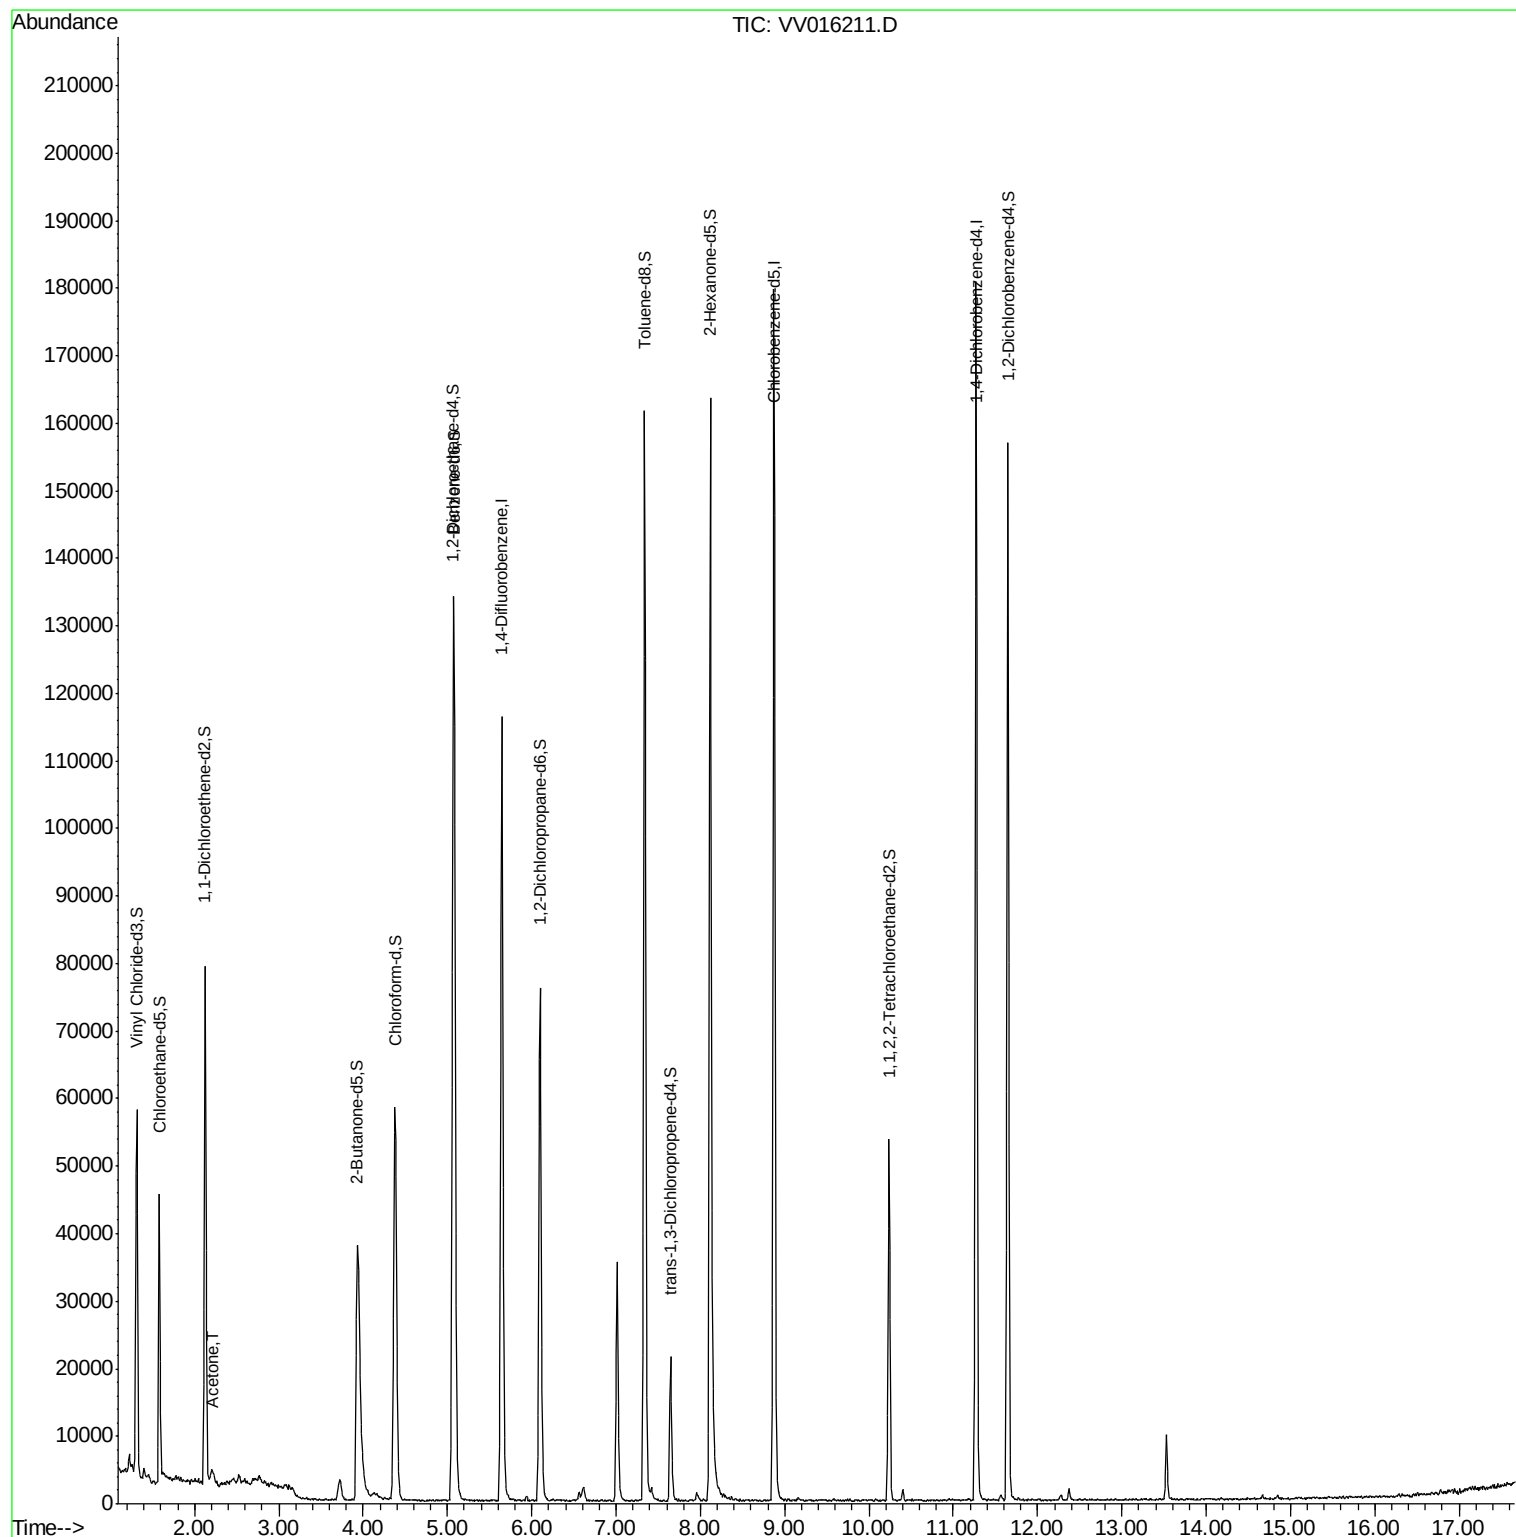

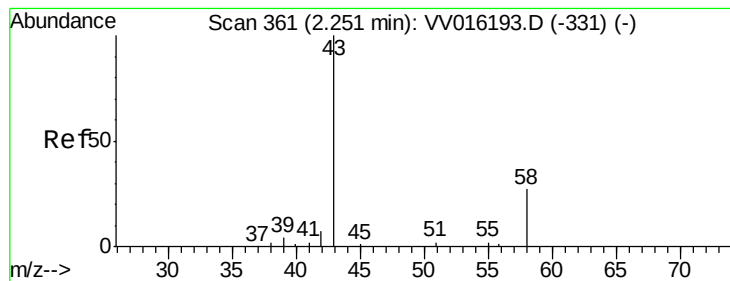

#13

Acetone

Concen: 3.906 ug/L

RT: 2.21 min Scan# 348

Delta R.T. -0.04 min

Lab File: VV016211.D

Acq: 26 May 2020 23:35

Instrument :
MSVOA_V
ClientSampleId :
GAXF7

Tot Ion: 43 Resp: 3603

Ion Ratio Lower Upper

43 100

58 25.8 0.0 48.8

