


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV052620\
 Data File : VV016190.D
 Acq On : 26 May 2020 14:14
 Operator : SY/MD
 Sample : BFB31
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB31

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR052620WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed May 27 03:06:56 2020

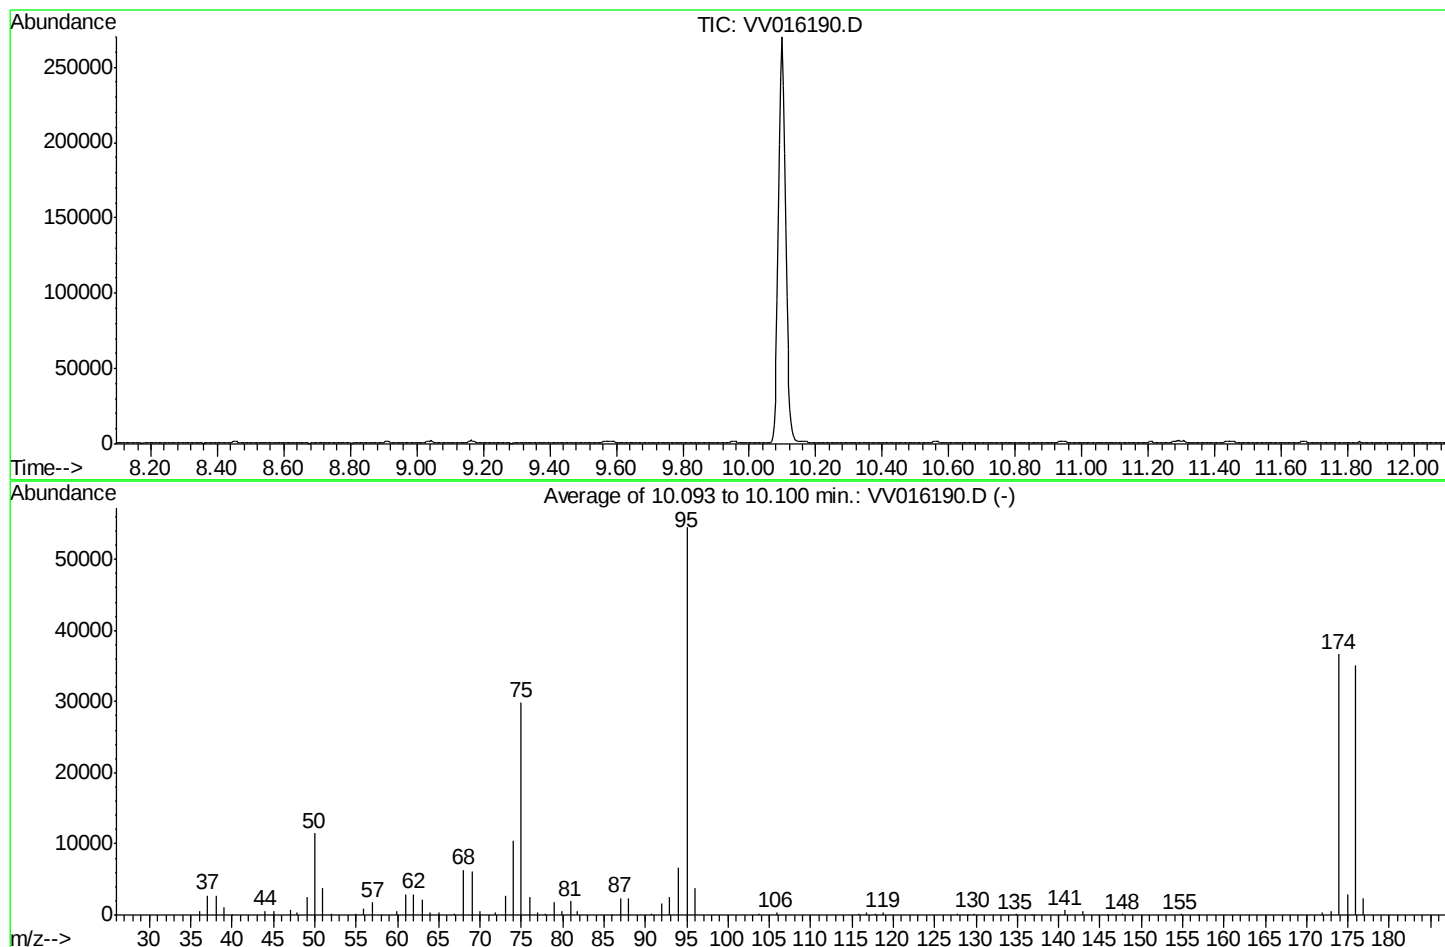

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	11497	PASS
75	95	30	80	54.7	29837	PASS
95	95	100	100	100.0	54514	PASS
96	95	5	9	7.1	3844	PASS
173	174	0.00	2	1.3	459	PASS
174	95	50	120	67.3	36696	PASS
175	174	5	9	8.0	2938	PASS
176	174	95	101	95.5	35050	PASS
177	176	5	9	6.9	2408	PASS

m/z	Abundance
36.00	626.0
37.00	2764.0
38.00	2615.0
39.00	1104.0
40.00	255.0
44.00	864.0
45.00	531.0
47.00	783.0
47.90	445.0
49.00	2338.0
50.00	11112.0
51.00	3643.0
51.90	163.0
54.90	205.0
55.90	814.0
57.00	1747.0
58.00	154.0
59.90	424.0
61.00	2849.0
62.00	2724.0
63.00	2087.0
63.90	293.0
65.00	293.0
67.00	193.0
68.00	6128.0
69.00	5877.0
69.90	468.0
71.90	435.0
73.00	2551.0
74.00	9722.0
75.00	28032.0
76.00	2430.0
76.90	358.0
78.00	213.0
78.90	1813.0
79.80	484.0
80.90	1774.0
81.80	445.0
87.00	2232.0
87.90	2092.0
90.80	208.0
91.90	1516.0
92.90	2303.0
94.00	6341.0
95.00	51144.0
96.00	3692.0
103.80	224.0
105.80	299.0
115.80	196.0
116.80	297.0
117.80	245.0
118.80	300.0
127.80	149.0
129.00	111.0
129.70	198.0
134.80	120.0
136.60	103.0
140.80	560.0
142.90	585.0
147.70	134.0
154.80	112.0
171.90	402.0
172.90	388.0
173.90	33552.0
174.90	2740.0
175.90	32168.0
176.90	2258.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31

m/z	Abundance
36.00	637.0
37.00	2845.0
38.00	2782.0
39.00	1168.0
40.00	253.0
44.00	919.0
45.00	578.0
47.00	843.0
47.90	461.0
49.00	2592.0
50.00	11909.0
51.00	3975.0
52.00	168.0
54.90	216.0
56.00	878.0
57.00	1808.0
58.00	133.0
59.90	464.0
61.00	3029.0
62.00	3072.0
63.00	2263.0
63.90	294.0
65.00	302.0
66.90	161.0
68.00	6696.0
69.00	6295.0
69.90	504.0
71.90	452.0
73.00	2839.0
74.00	10758.0
75.00	30912.0
76.00	2523.0
76.90	392.0
77.80	218.0
78.90	1945.0
79.80	595.0
80.90	1970.0
81.80	542.0
85.90	115.0
87.00	2443.0
87.90	2324.0
90.80	189.0
91.90	1601.0
93.00	2591.0
94.00	6921.0
95.00	56336.0
96.00	4012.0
103.80	253.0
105.90	325.0
115.70	206.0
116.80	354.0
117.70	286.0
118.80	345.0
127.80	204.0
129.00	103.0
129.80	198.0
134.90	131.0
136.70	107.0
137.00	106.0
140.80	693.0
142.90	624.0
147.80	141.0
154.80	144.0
156.80	105.0
171.80	373.0
172.90	456.0
173.90	38000.0
174.90	3068.0
175.90	36344.0
176.90	2541.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31

m/z	Abundance
36.00	570.0
37.00	2701.0
38.00	2691.0
39.00	1124.0
40.00	272.0
44.00	819.0
45.00	551.0
47.00	764.0
47.90	393.0
49.00	2604.0
50.00	11471.0
51.00	3709.0
52.00	168.0
54.90	201.0
56.00	857.0
57.00	1741.0
59.90	497.0
61.00	2942.0
62.00	3125.0
63.00	2240.0
63.90	271.0
65.00	302.0
66.80	146.0
68.00	6315.0
69.00	5998.0
69.90	495.0
71.90	409.0
73.00	2831.0
74.00	10597.0
75.00	30568.0
76.00	2476.0
76.90	397.0
77.80	202.0
78.90	1916.0
79.90	668.0
80.90	2028.0
81.80	561.0
85.90	120.0
86.90	2422.0
87.90	2364.0
90.80	186.0
91.90	1586.0
93.00	2553.0
94.00	6963.0
95.00	56064.0
96.00	3828.0
103.80	265.0
105.90	347.0
115.70	214.0
116.80	366.0
117.70	292.0
118.80	381.0
127.80	223.0
129.80	207.0
134.80	121.0
137.00	111.0
140.80	671.0
142.90	613.0
145.80	102.0
147.80	116.0
154.80	128.0
156.80	102.0
171.90	298.0
173.00	534.0
173.90	38536.0
174.90	3006.0
175.90	36640.0
176.90	2425.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31

Scan 2788 (10.055 min): VV016190.D
BFB31

m/z	Abundance
39.90	218.0
44.00	313.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31