




Quantitation Report (Qedit)

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV052621\  
 Data File : VV021420.D  
 Acq On : 26 May 2021 13:02  
 Operator : SY/MD  
 Sample : M2496-20  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
 MSVOA\_V  
**ClientSampleId :**  
 GB460

**Manual Integrations**  
**APPROVED**  
 MMDadoda  
 5/28/2021 11:27:10 AM

Quant Time: May 27 02:04:41 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR052521WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu May 27 02:03:26 2021  
 Response via : Initial Calibration

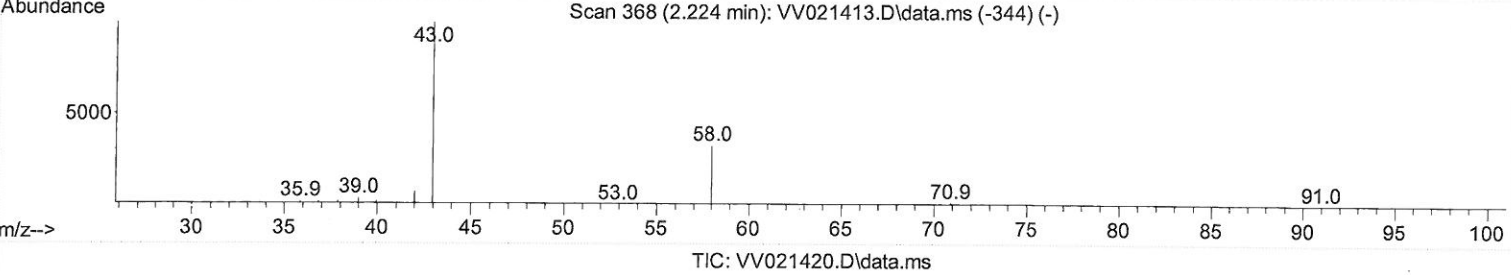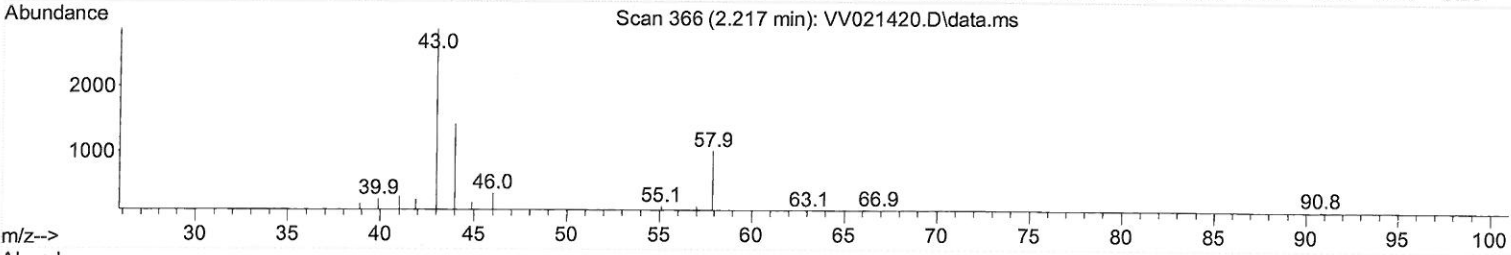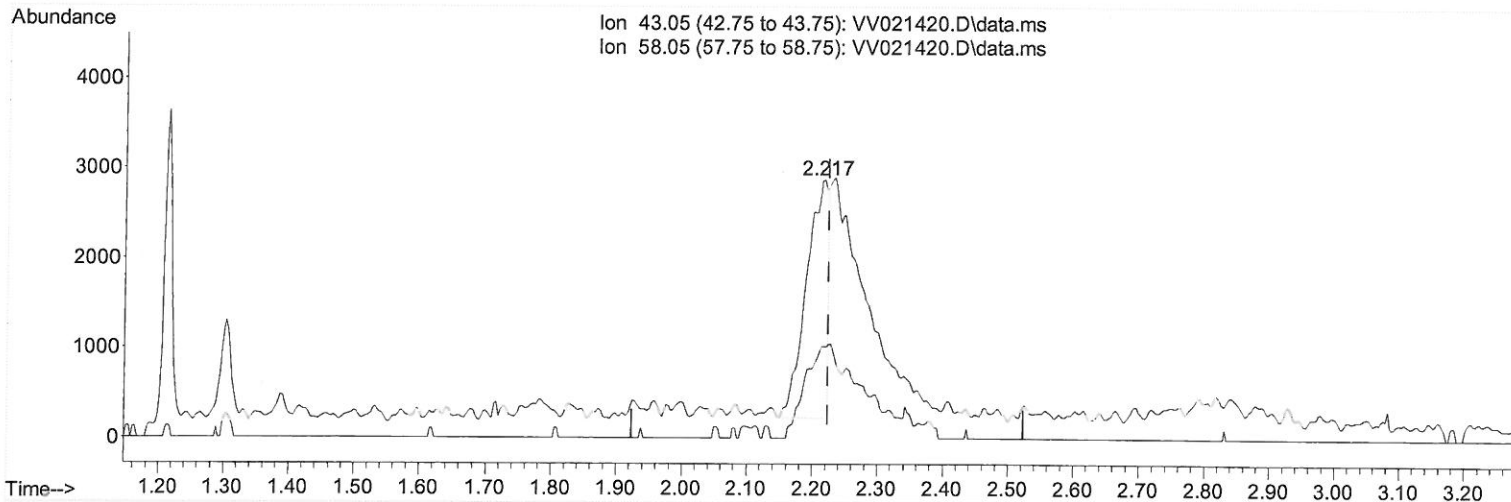

(13) Acetone (T)  
 2.217min (-0.006) 3.19 ug/L

response	6248
Ion	Exp% Act%
43.05	100.00 100.00
58.05	9.30 58.03#
0.00	0.00 0.00
0.00	0.00 0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV052621\  
 Data File : VV021420.D  
 Acq On : 26 May 2021 13:02  
 Operator : SY/MD  
 Sample : M2496-20  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampled :  
 GB460

Manual Integrations  
 APPROVED

MMDadoda  
 5/28/2021 11:27:10 AM

Quant Time: May 27 02:04:41 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR052521WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu May 27 02:03:26 2021  
 Response via : Initial Calibration

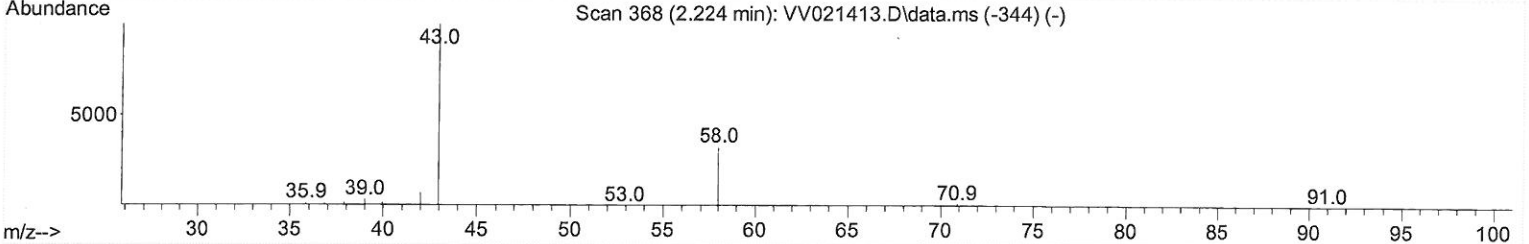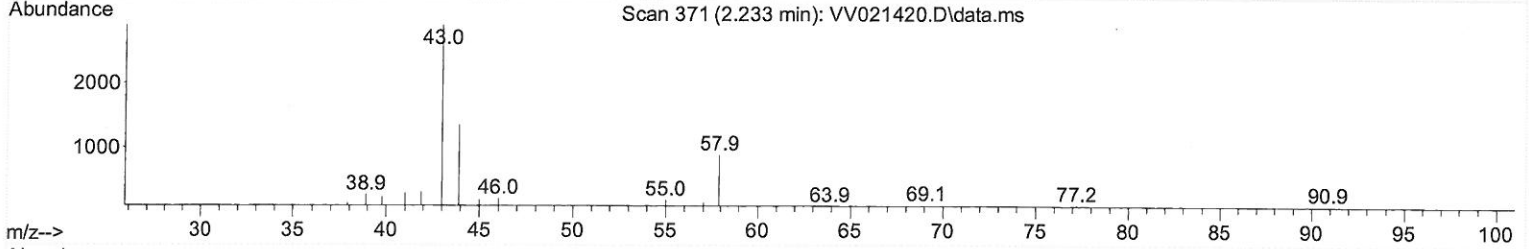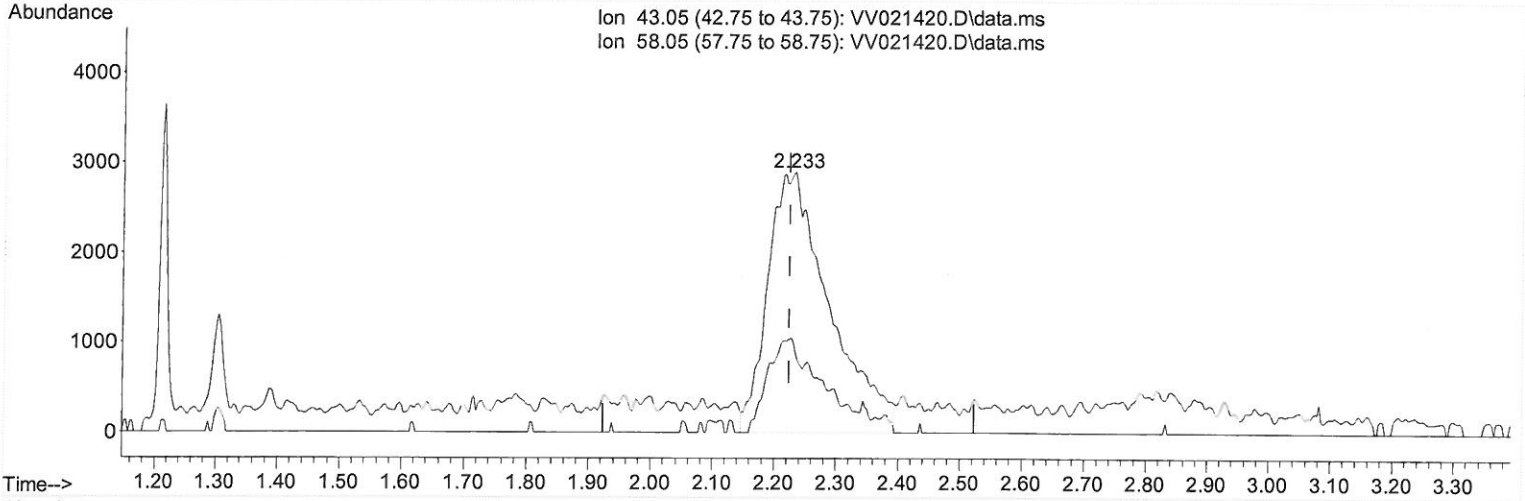

TIC: VV021420.D\data.ms

(13) Acetone (T)

2.233min (+ 0.010) 10.20 ug/L m

06/02/2154

response 19967

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	9.30	18.16
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW052621\  
 Data File : VW021420.D  
 Acq On : 26 May 2021 13:02  
 Operator : SY/MD  
 Sample : M2496-20  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
 MSVOA\_V  
**Client Sampled :**  
 GB460

**Manual Integrations**  
**APPROVED**  
 MMDadoda  
 5/28/2021 11:27:10 AM

Quant Time: May 27 02:04:41 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR052521WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu May 27 02:03:26 2021  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----						
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	228400	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	214543	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	121076	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	42972	4.45	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	89.00%	
7) Chloroethane-d5	1.564	69	44517	4.83	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	96.60%	
11) 1,1-Dichloroethene-d2	2.105	63	58485	3.19	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	63.80%	
20) 2-Butanone-d5	3.918	46	205440	59.14	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	118.28%	
24) Chloroform-d	4.352	84	129714	4.84	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.80%	
26) 1,2-Dichloroethane-d4	5.037	65	66174	5.37	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	107.40%	
32) Benzene-d6	5.053	84	250595	4.85	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.00%	
36) 1,2-Dichloropropane-d6	6.076	67	82452	4.93	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	98.60%	
41) Toluene-d8	7.320	98	228595	4.83	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.60%	
43) trans-1,3-Dichloroprop...	7.629	79	33521	4.81	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	96.20%	
46) 2-Hexanone-d5	8.092	63	190415	58.04	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	116.08%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	69034	5.12	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	102.40%	
66) 1,2-Dichlorobenzene-d4	11.625	152	105312	5.05	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	101.00%	
-----						
Target Compounds						
13) Acetone	2.233	43	19967m)	10.20	ug/L	Qvalue 06/02/21 57
25) Chloroform	4.381	83	37897	1.48	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW052621\  
Data File : VW021420.D  
Acq On : 26 May 2021 13:02  
Operator : SY/MD  
Sample : M2496-20  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
Client Sampled :  
GB460

Manual Integrations  
APPROVED  
MMDadoda  
5/28/2021 11:27:10 AM

Quant Time: May 27 02:04:41 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR052521WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Thu May 27 02:03:26 2021  
Response via : Initial Calibration

