

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052621\
 Data File : VV021433.D
 Acq On : 26 May 2021 18:09
 Operator : SY/MD
 Sample : M2496-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: May 27 02:06:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu May 27 02:03:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	233436	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	216426	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	120631	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	42479	4.30	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.00%
7) Chloroethane-d5	1.568	69	45660	4.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.80%
11) 1,1-Dichloroethene-d2	2.108	63	59295	3.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.40%
20) 2-Butanone-d5	3.918	46	208681	58.78	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.56%
24) Chloroform-d	4.352	84	131981	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.40%
26) 1,2-Dichloroethane-d4	5.037	65	66483	5.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.60%
32) Benzene-d6	5.053	84	254411	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
36) 1,2-Dichloropropane-d6	6.072	67	83712	4.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.20%
41) Toluene-d8	7.320	98	230697	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
43) trans-1,3-Dichloroprop...	7.628	79	33058	4.70	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.00%
46) 2-Hexanone-d5	8.091	63	185019	55.91	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.82%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	69658	5.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.40%
66) 1,2-Dichlorobenzene-d4	11.625	152	106254	5.11	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.20%
Target Compounds						
16) Methylene chloride	2.510	84	13016	0.68	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052621\
Data File : VV021433.D
Acq On : 26 May 2021 18:09
Operator : SY/MD
Sample : M2496-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: May 27 02:06:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu May 27 02:03:26 2021
Response via : Initial Calibration

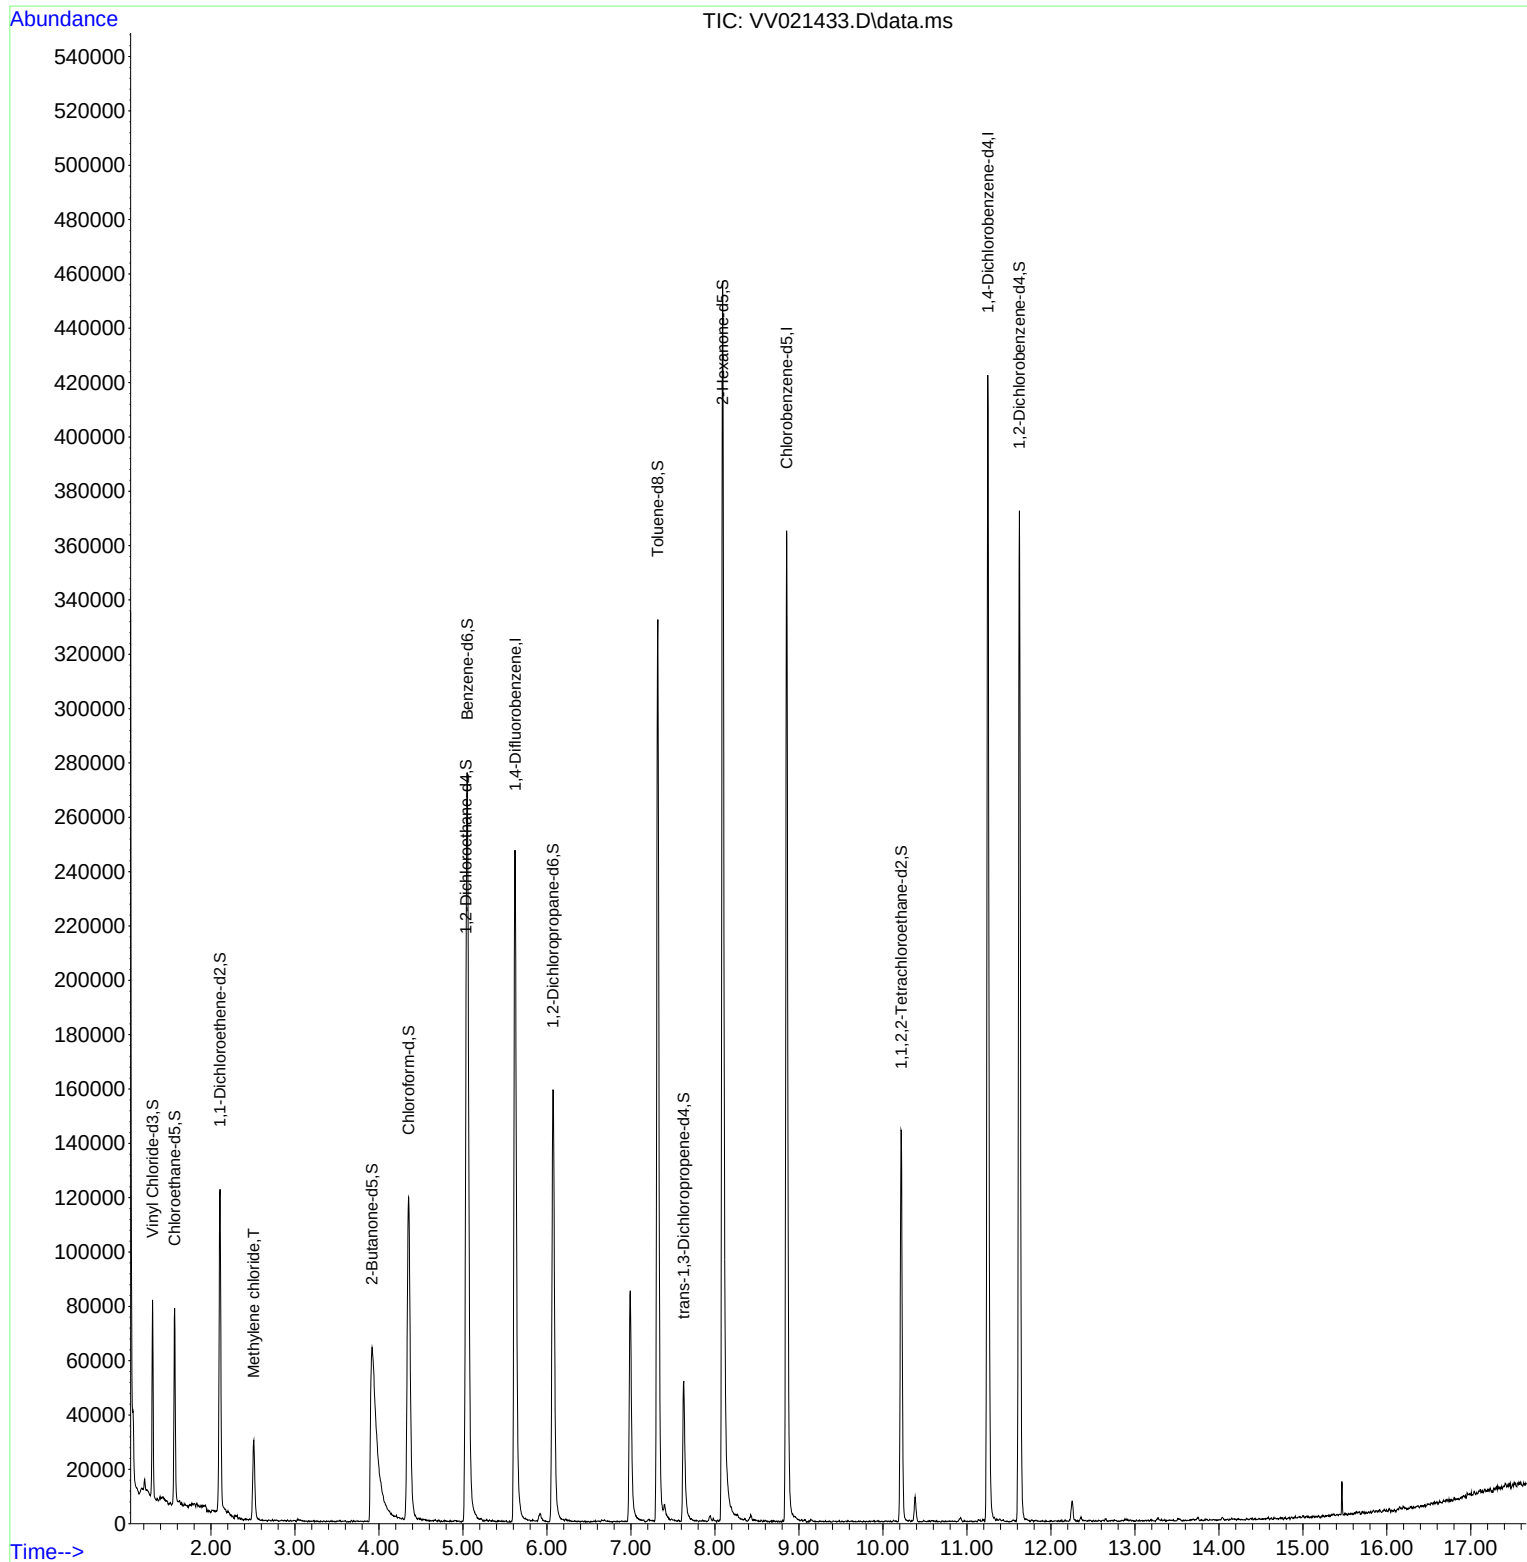

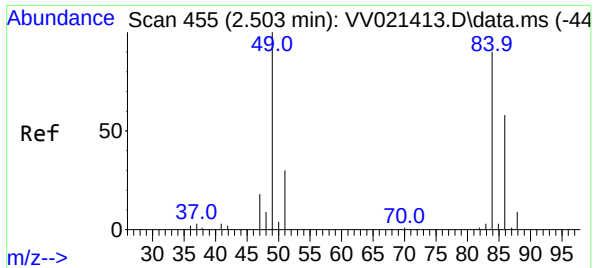

#16
Methylene chloride
Concen: 0.68 ug/L
RT: 2.510 min Scan# 457
Delta R.T. 0.006 min
Lab File: VV021433.D
Acq: 26 May 2021 18:09

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

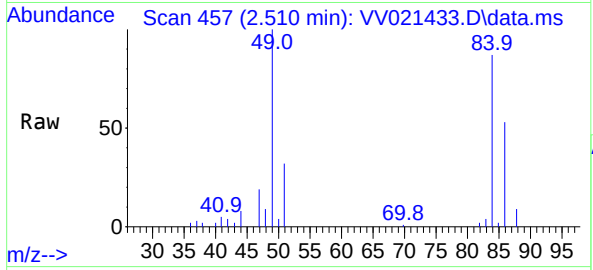

Tgt Ion:	84	Resp:	13016
Ion	Ratio	Lower	Upper
84	100		
86	60.5	44.7	82.9
49	114.9	82.7	153.5

