

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052621\
 Data File : VV021434.D
 Acq On : 26 May 2021 18:33
 Operator : SY/MD
 Sample : M2528-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: May 27 02:06:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu May 27 02:03:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	224320	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	214017	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	117171	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	40255	4.24	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.80%
7) Chloroethane-d5	1.568	69	42402	4.68	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.60%
11) 1,1-Dichloroethene-d2	2.105	63	57158	3.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.60%
20) 2-Butanone-d5	3.912	46	183293	53.73	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.46%
24) Chloroform-d	4.352	84	121633	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.40%
26) 1,2-Dichloroethane-d4	5.037	65	61389	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.40%
32) Benzene-d6	5.053	84	239755	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.20%
36) 1,2-Dichloropropane-d6	6.072	67	76855	4.60	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.00%
41) Toluene-d8	7.320	98	215687	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
43) trans-1,3-Dichloroprop...	7.629	79	30848	4.44	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.80%
46) 2-Hexanone-d5	8.092	63	166862	50.99	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.98%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	64201	4.77	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.40%
66) 1,2-Dichlorobenzene-d4	11.625	152	98849	4.89	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.80%
Target Compounds						
16) Methylene chloride	2.507	84	11131	0.61	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052621\
Data File : VV021434.D
Acq On : 26 May 2021 18:33
Operator : SY/MD
Sample : M2528-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: May 27 02:06:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu May 27 02:03:26 2021
Response via : Initial Calibration

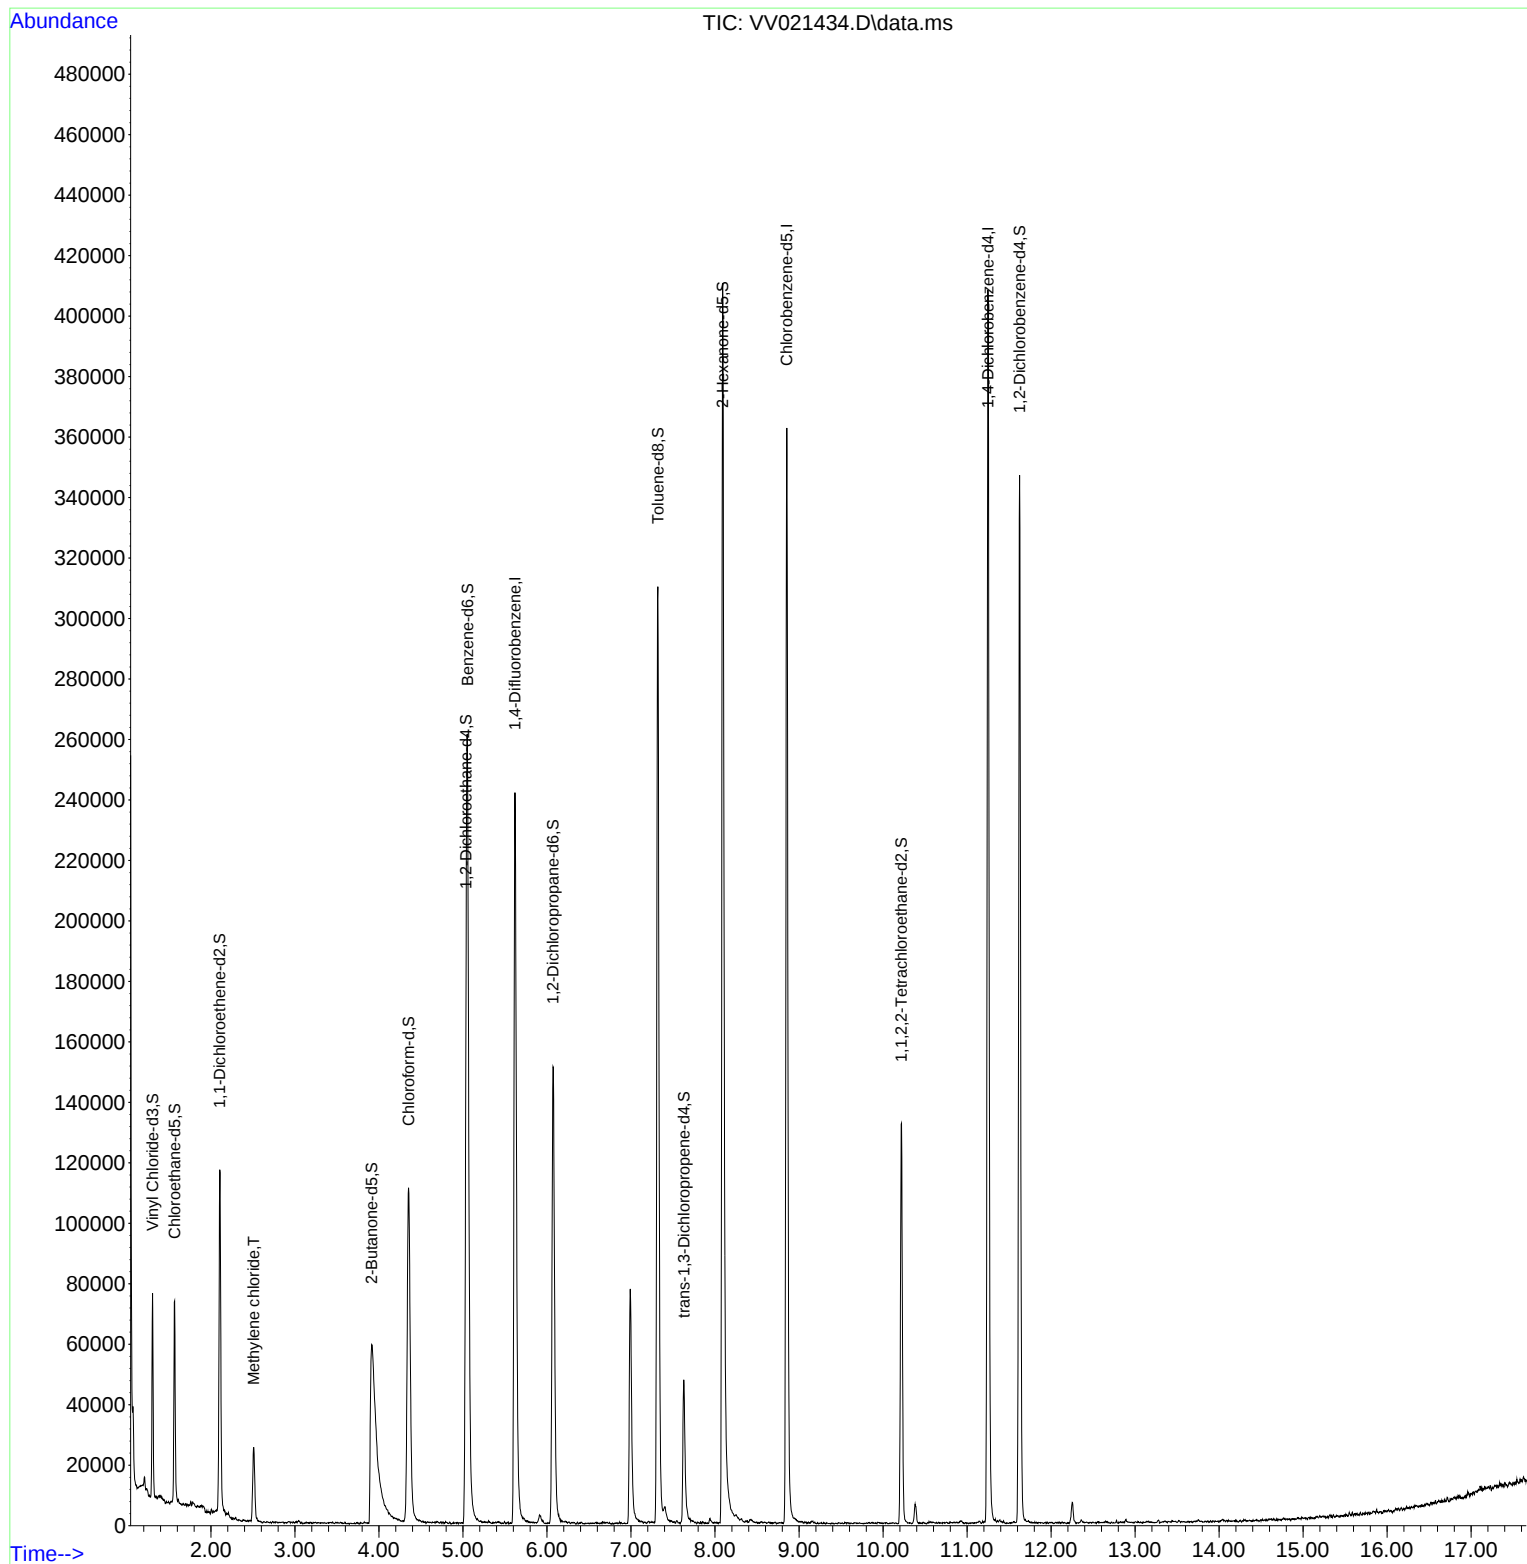

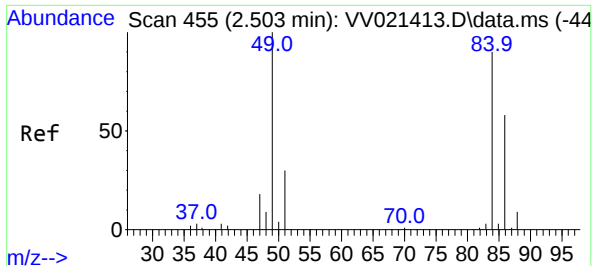

#16
Methylene chloride
Concen: 0.61 ug/L
RT: 2.507 min Scan# 456
Delta R.T. 0.003 min
Lab File: VV021434.D
Acq: 26 May 2021 18:33

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

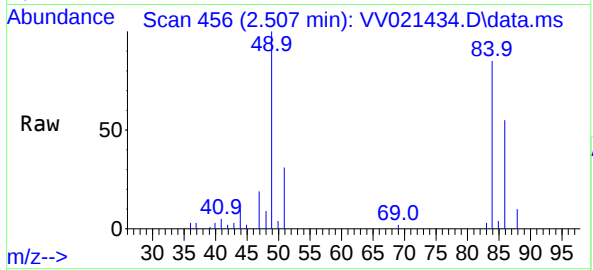

Tgt Ion:	84	Resp:	11131
Ion	Ratio	Lower	Upper
84	100		
86	65.1	44.7	82.9
49	118.0	82.7	153.5

