

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052621\
 Data File : VV021432.D
 Acq On : 26 May 2021 17:45
 Operator : SY/MD
 Sample : VIBLK170
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK170

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV021432.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	93	rVB	65035	66037	8.37%	1.086%
2	1.568	157	164	176	rVB	68347	78456	9.95%	1.290%
3	2.108	322	332	349	rVB	117146	169181	21.45%	2.781%
4	2.510	446	457	470	rBV	23588	39309	4.98%	0.646%
5	3.905	880	891	942	rBV	77429	317938	40.31%	5.226%
6	4.352	1013	1030	1056	rBV	113319	284764	36.11%	4.681%
7	5.050	1230	1247	1277	rBV2	262094	655190	83.07%	10.770%
8	5.619	1412	1424	1451	rBV	242426	495758	62.86%	8.149%
9	6.072	1550	1565	1584	rBV	151072	313645	39.77%	5.156%
10	6.992	1839	1851	1876	rBV2	78905	155458	19.71%	2.555%
11	7.320	1941	1953	1972	rBV	317858	555897	70.48%	9.138%
12	7.628	2039	2049	2077	rBV	47720	90045	11.42%	1.480%
13	7.944	2138	2147	2156	rBV3	6345	10599	1.34%	0.174%
14	8.091	2179	2193	2230	rBV	437692	788688	100.00%	12.964%
15	8.854	2418	2430	2450	rBV	353111	587624	74.51%	9.659%
16	10.217	2841	2854	2870	rBV	134906	216727	27.48%	3.563%
17	10.384	2892	2906	2919	rBV	16646	27210	3.45%	0.447%
18	11.249	3164	3175	3199	rBV	416839	650374	82.46%	10.691%
19	11.625	3280	3292	3314	rBV	355496	564233	71.54%	9.275%
20	12.252	3475	3487	3498	rBV	10200	16355	2.07%	0.269%




Sum of corrected areas: 6083488

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052621\
Data File : VV021432.D
Acq On : 26 May 2021 17:45
Operator : SY/MD
Sample : VIBLK170
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK170

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

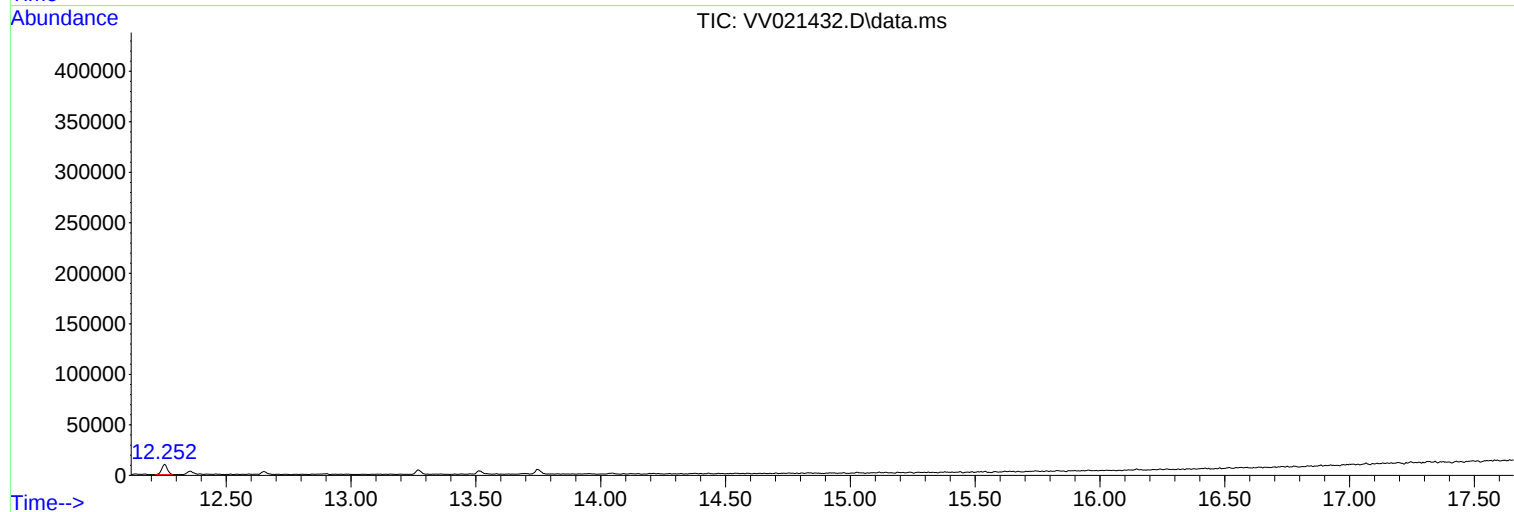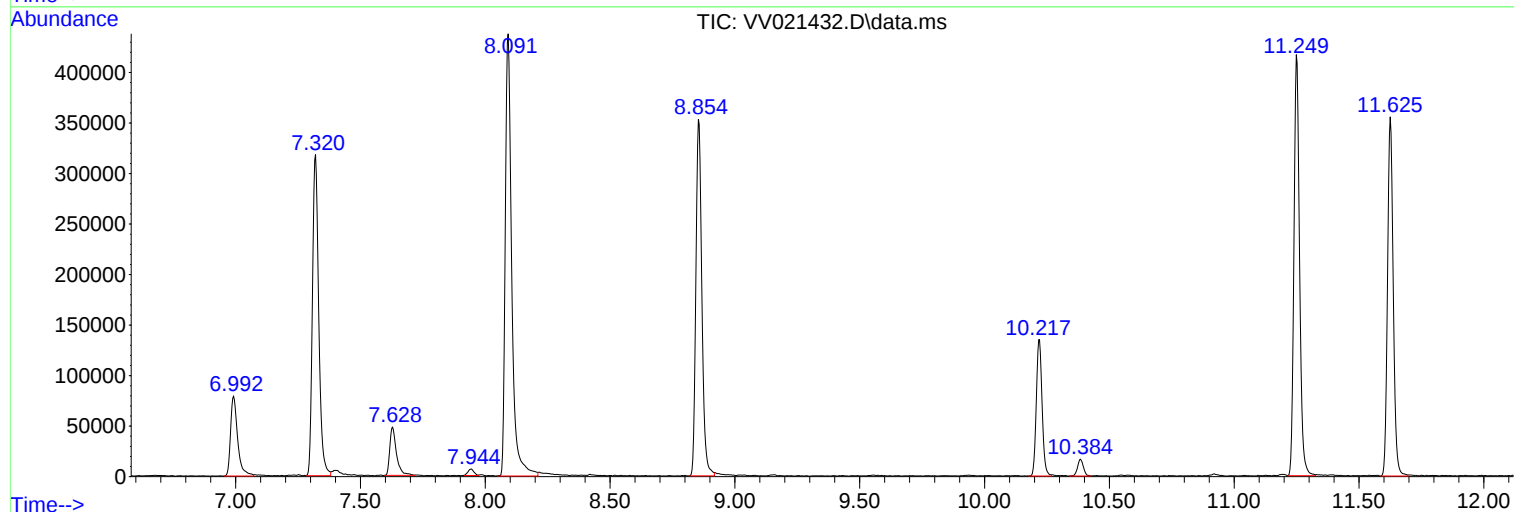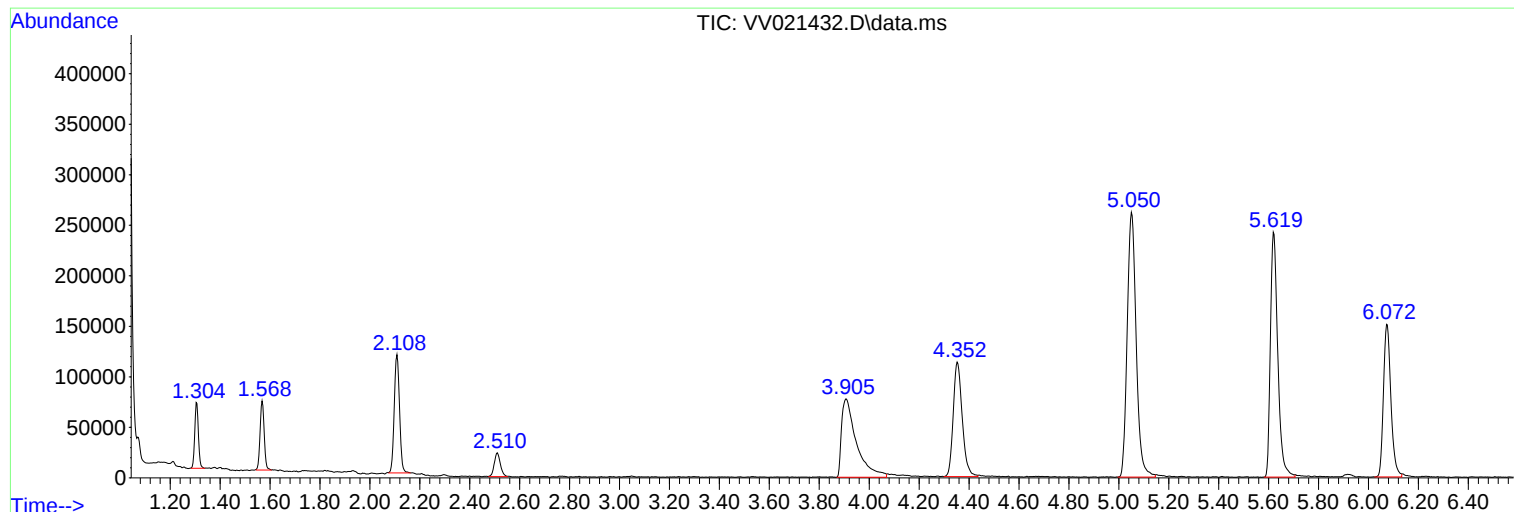

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052621\
Data File : VV021432.D
Acq On : 26 May 2021 17:45
Operator : SY/MD
Sample : VIBLK170
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK170

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052621\
Data File : VV021432.D
Acq On : 26 May 2021 17:45
Operator : SY/MD
Sample : VIBLK170
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK170

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
