
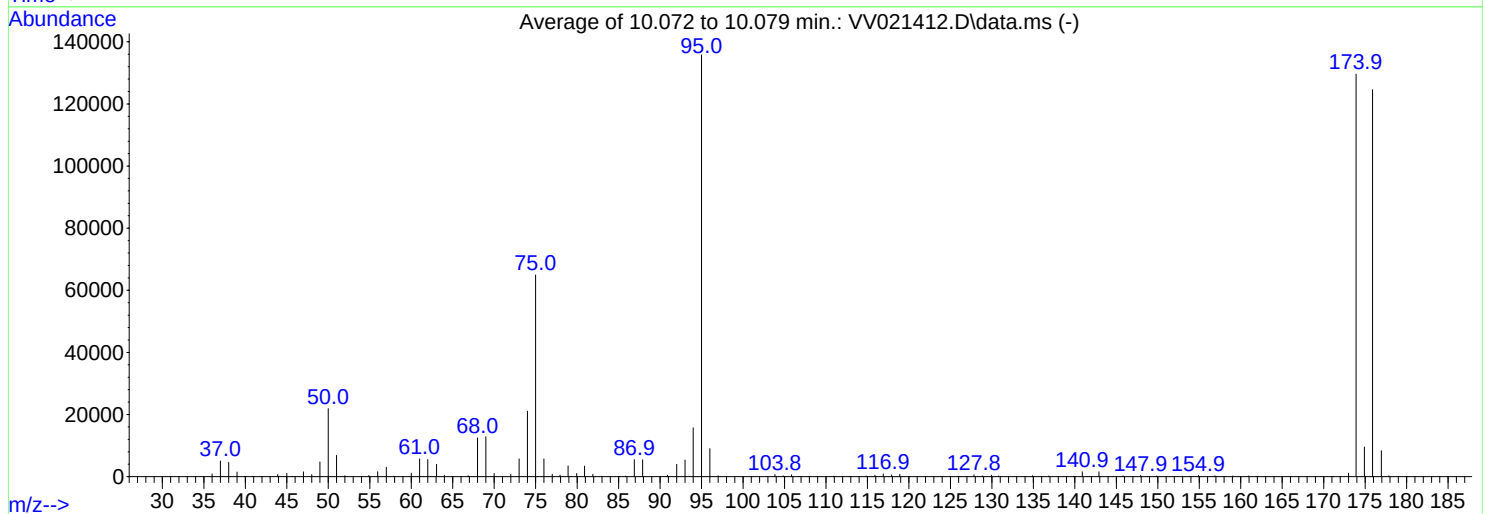


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052621\
 Data File : VV021412.D
 Acq On : 26 May 2021 08:57
 Operator : SY/MD
 Sample : BFB62
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB162

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu May 27 02:03:26 2021

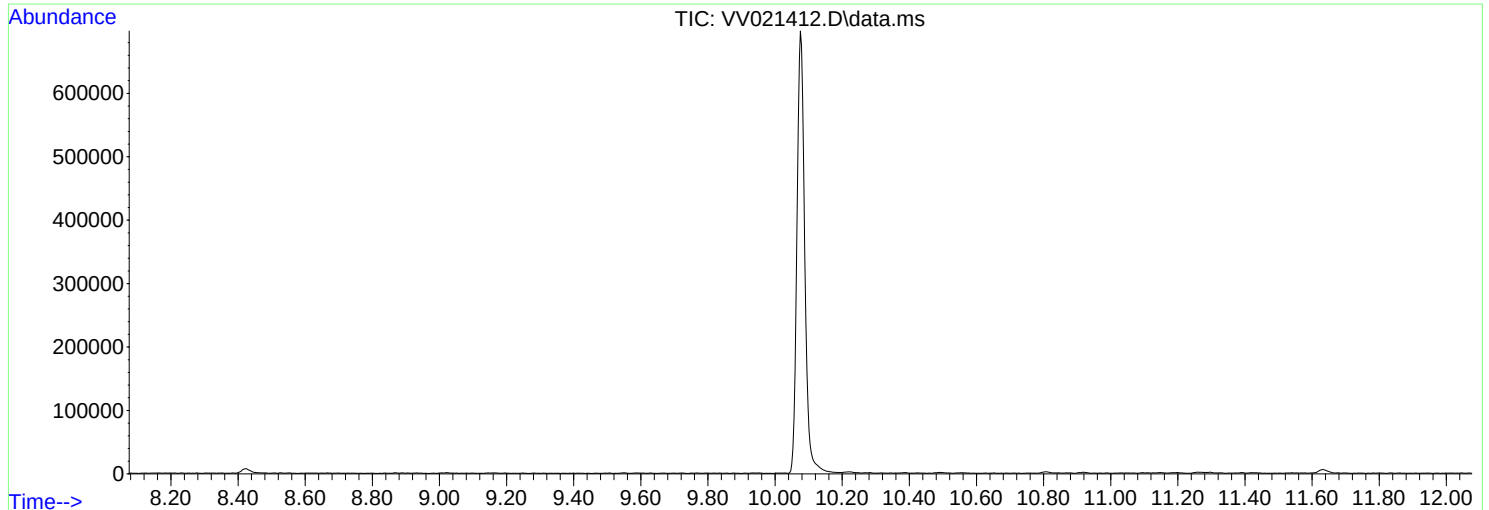

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	21896	PASS
75	95	30	80	47.8	64933	PASS
95	95	100	100	100.0	135808	PASS
96	95	5	9	6.6	9012	PASS
173	174	0.00	2	0.9	1157	PASS
174	95	50	120	95.4	129611	PASS
175	174	5	9	7.3	9519	PASS
176	174	95	105	96.1	124579	PASS
177	176	5	10	6.7	8342	PASS

m/z	Abundance
36.00	880.0
37.00	5127.0
38.00	4502.0
39.00	1631.0
40.10	206.0
40.90	147.0
41.90	141.0
43.00	238.0
44.00	1184.0
45.00	1033.0
45.70	148.0
47.00	1536.0
48.00	649.0
49.00	4643.0
50.00	21472.0
51.00	6844.0
52.00	355.0
54.90	537.0
56.00	1439.0
57.00	2950.0
57.90	175.0
60.00	1070.0
61.00	5725.0
62.00	5326.0
63.10	3899.0
64.00	416.0
66.90	310.0
68.00	12146.0
69.00	12745.0
70.00	1054.0
72.00	749.0
73.00	5602.0
74.00	20648.0
75.00	64144.0
76.00	5583.0
77.00	809.0
77.90	506.0
78.90	3308.0
79.90	904.0
80.90	3305.0
81.90	788.0
83.00	130.0
85.90	202.0
86.90	5462.0
87.90	5344.0
90.90	480.0
92.00	3833.0
93.00	5175.0
94.00	15311.0
95.00	132992.0
96.00	8791.0
97.00	256.0
103.80	637.0
104.90	266.0
105.90	608.0
110.90	154.0
112.90	159.0
114.90	171.0
115.90	428.0
116.90	859.0
117.90	502.0
118.90	739.0
123.80	110.0
127.90	526.0
128.90	249.0
130.00	462.0
130.80	190.0
134.90	271.0
137.00	218.0
140.90	1475.0
141.80	215.0
142.90	1485.0
145.80	238.0
147.90	349.0
148.80	108.0
149.80	202.0
153.00	183.0
154.90	340.0
156.90	250.0
159.00	212.0
161.00	195.0
171.20	115.0
173.00	1111.0
173.90	123168.0
174.90	9495.0
175.90	118480.0
177.00	8116.0
177.90	246.0

Instrument :
MSVOA_V
ClientSampleId :
BFB162

m/z	Abundance
36.00	912.0
37.00	5220.0
38.00	4761.0
39.00	1687.0
40.00	233.0
40.90	118.0
43.00	244.0
44.00	1174.0
45.00	1095.0
45.70	134.0
47.00	1586.0
48.00	651.0
49.00	4970.0
50.00	22552.0
51.00	7090.0
52.00	311.0
54.90	543.0
56.00	1603.0
57.00	3154.0
57.90	168.0
60.00	1193.0
61.00	5950.0
62.00	5679.0
63.00	4114.0
64.00	417.0
66.80	339.0
68.00	12912.0
69.00	13272.0
70.00	1093.0
72.00	768.0
73.00	5993.0
74.00	21584.0
75.00	67080.0
76.00	5945.0
77.00	823.0
77.90	535.0
78.90	3571.0
79.90	1064.0
80.90	3490.0
81.90	821.0
82.90	177.0
85.90	207.0
86.90	5594.0
87.90	5570.0
90.90	500.0
92.00	4071.0
93.00	5564.0
94.00	16189.0
95.00	140224.0
96.00	9360.0
97.00	304.0
103.90	698.0
104.80	284.0
105.80	652.0
110.90	189.0
112.80	136.0
114.80	207.0
115.90	456.0
116.90	895.0
117.90	580.0
118.90	823.0
123.80	116.0
127.80	568.0
128.80	274.0
129.90	473.0
130.80	222.0
134.90	346.0
136.80	227.0
139.80	137.0
140.90	1614.0
141.80	182.0
142.90	1597.0
145.00	106.0
145.80	274.0
147.90	401.0
148.70	102.0
149.90	207.0
153.00	190.0
153.80	105.0
154.90	366.0
156.90	282.0
159.10	240.0
160.90	231.0
171.20	120.0
173.00	1174.0
173.90	133824.0
174.90	9850.0
175.90	128576.0
177.00	8611.0
177.90	273.0

Instrument :
MSVOA_V
ClientSampleId :
BFB162

m/z	Abundance
36.00	877.0
37.00	4877.0
38.00	4466.0
39.00	1637.0
40.00	286.0
43.00	230.0
43.90	1067.0
45.00	1116.0
45.70	104.0
47.00	1507.0
48.00	671.0
49.00	4641.0
50.00	21664.0
51.00	6608.0
52.00	241.0
55.00	454.0
55.90	1693.0
57.00	3061.0
57.90	147.0
60.00	1116.0
61.00	5468.0
62.00	5505.0
63.00	3975.0
64.00	375.0
66.80	372.0
68.00	12316.0
69.00	12530.0
70.00	1027.0
72.00	683.0
73.00	5651.0
74.00	20944.0
75.00	63576.0
76.00	5590.0
77.00	763.0
78.00	550.0
78.90	3457.0
80.00	1097.0
80.90	3398.0
81.90	776.0
82.90	210.0
85.80	173.0
86.90	5402.0
87.90	5261.0
90.90	465.0
92.00	3983.0
93.00	5288.0
94.00	15656.0
95.00	134208.0
96.00	8885.0
97.00	287.0
103.90	692.0
104.80	256.0
105.80	608.0
106.70	110.0
110.90	185.0
112.80	111.0
114.80	209.0
115.90	482.0
116.90	839.0
117.90	593.0
118.90	808.0
123.90	128.0
127.80	547.0
128.80	266.0
129.90	489.0
130.80	201.0
134.90	356.0
136.80	235.0
139.90	150.0
140.90	1562.0
142.10	138.0
142.90	1503.0
145.00	139.0
145.80	247.0
148.00	441.0
148.70	101.0
149.90	202.0
153.00	120.0
153.90	116.0
154.90	370.0
156.90	250.0
159.10	232.0
160.90	246.0
172.00	222.0
173.00	1186.0
173.90	131840.0
174.90	9212.0
175.90	126680.0
176.90	8299.0
177.80	277.0

Instrument :
MSVOA_V
ClientSampleId :
BFB162

m/z	Abundance
39.00	137.0
39.90	216.0
42.90	164.0
43.90	472.0
54.90	131.0
56.20	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB162