

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052623\
 Data File : VV031245.D
 Acq On : 26 May 2023 10:02
 Operator : SY/MD
 Sample : VV0526MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: May 27 00:52:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat May 27 00:51:17 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	300827	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	284869	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	147501	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	135039	52.525	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	105.060%	
7) Chloroethane-d5	1.536	69	101386	51.190	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	102.380%	
11) 1,1-Dichloroethene-d2	2.066	65	51516	42.731	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	85.460%	
21) 2-Butanone-d5	3.799	46	176006	128.480	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	128.480%	
24) Chloroform-d	4.259	84	246806	54.265	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	108.520%	
26) 1,2-Dichloroethane-d4	4.950	65	170812	55.578	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	111.160%	
32) Benzene-d6	4.970	84	435277	56.364	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	112.720%	
36) 1,2-Dichloropropane-d6	5.995	67	138087	59.761	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	119.520%	
41) Toluene-d8	7.249	98	297162	41.229	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	82.460%	
43) trans-1,3-Dichloroprop...	7.558	79	57613	49.697	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	99.400%	
47) 2-Hexanone-d5	8.034	63	105873	117.517	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	117.520%	
56) 1,1,2,2-Tetrachloroeth...	10.159	84	182964	52.793	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	105.580%	
66) 1,2-Dichlorobenzene-d4	11.567	152	144858	54.651	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	109.300%	
Target Compounds						
44) trans-1,3-Dichloropropene	7.555	75	2751	0.939	ug/L	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052623\
Data File : VV031245.D
Acq On : 26 May 2023 10:02
Operator : SY/MD
Sample : VV0526MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: May 27 00:52:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 27 00:51:17 2023
Response via : Initial Calibration

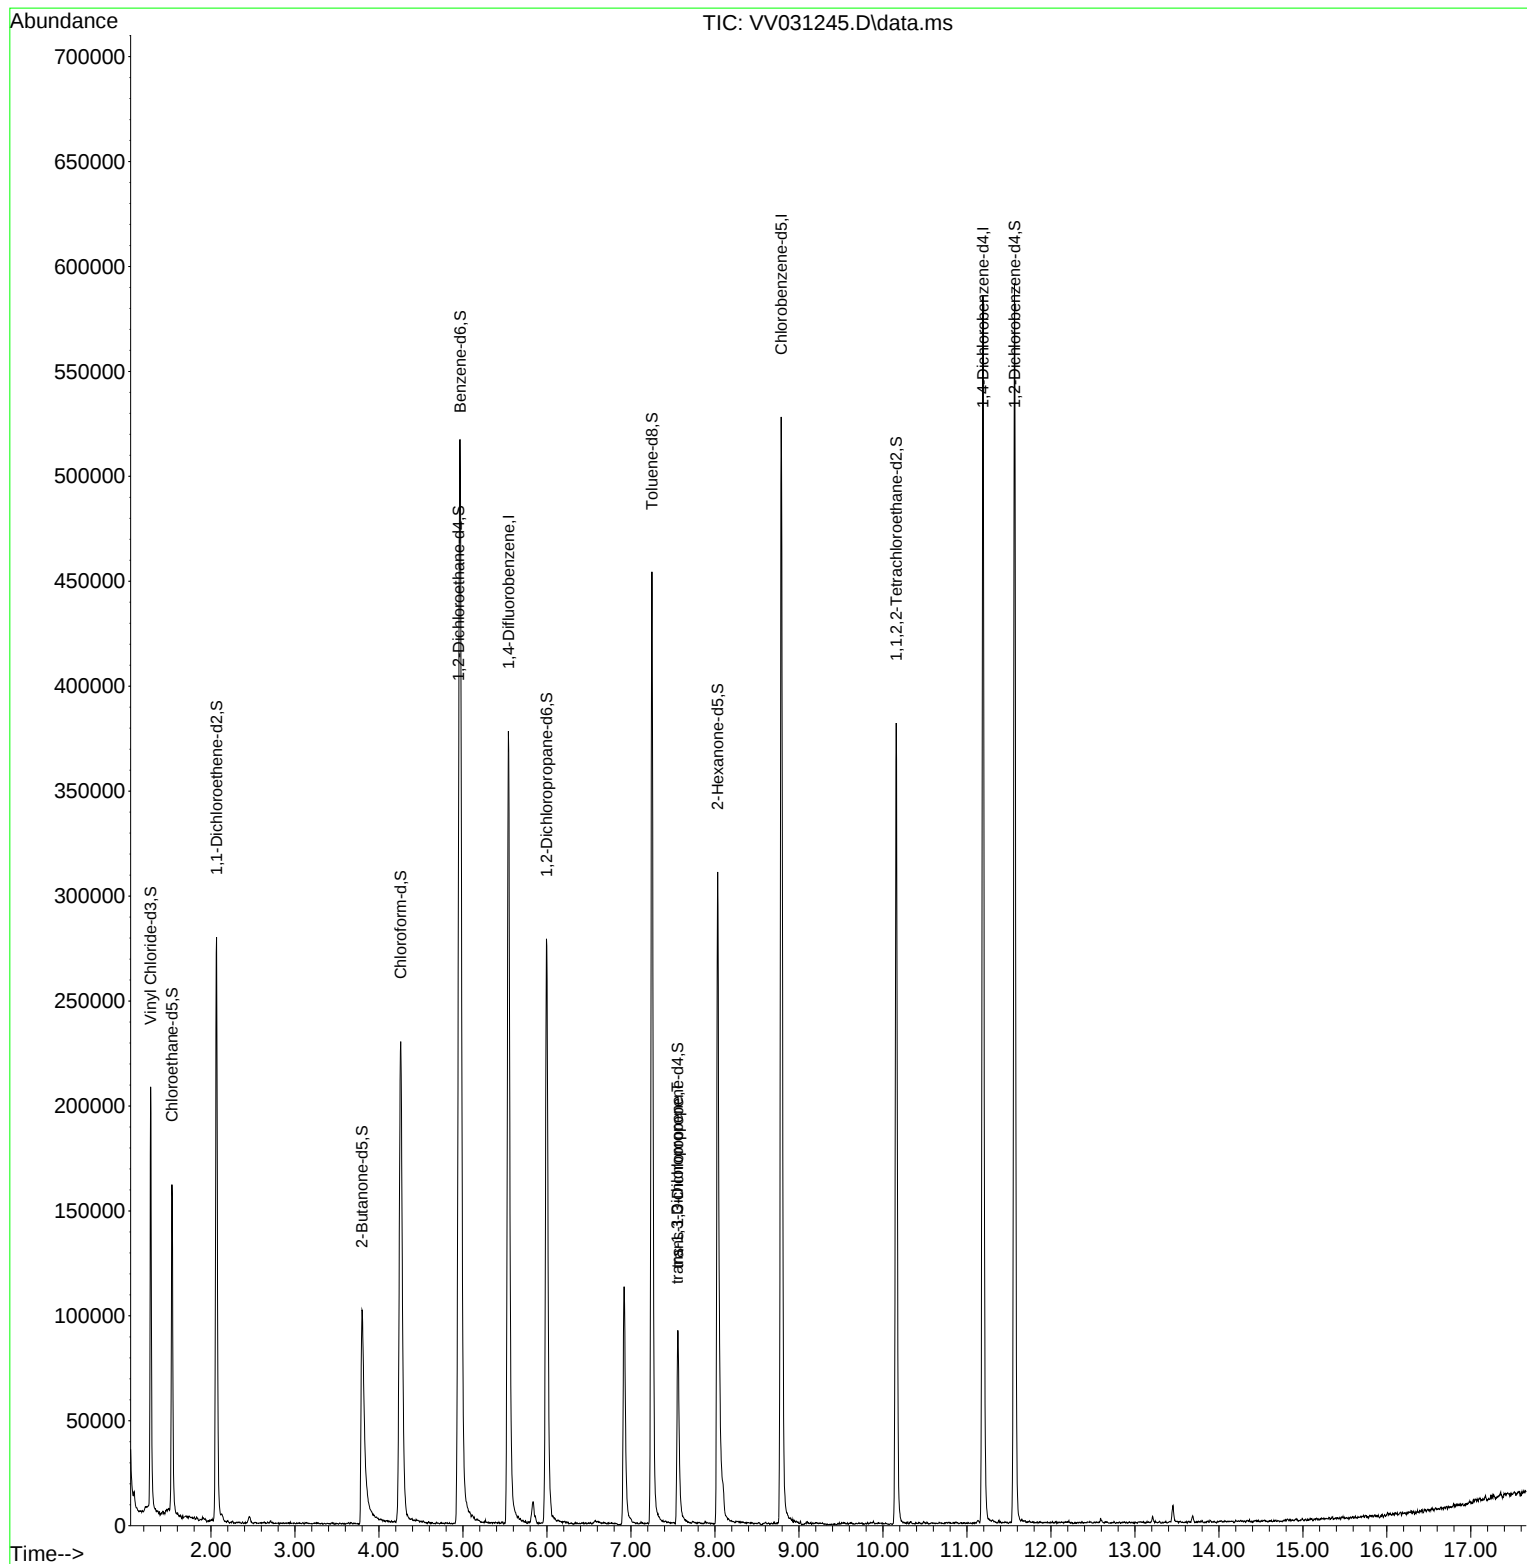

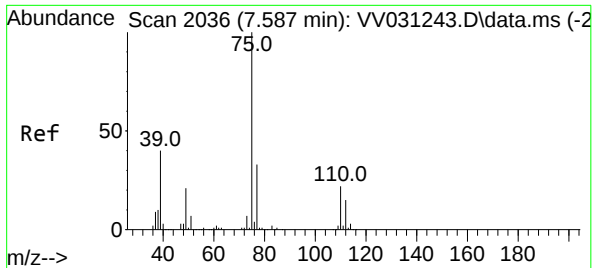

#44
 trans-1,3-Dichloropropene
 Concen: 0.939 ug/L
 RT: 7.555 min Scan# 2036
 Delta R.T. -0.032 min
 Lab File: VV031245.D
 Acq: 26 May 2023 10:02

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 2751
 Ion Ratio Lower Upper
 75 100
 77 40.2 22.2 41.2

