

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052623\
 Data File : VV031244.D
 Acq On : 26 May 2023 09:39
 Operator : SY/MD
 Sample : VV0526MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK345

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031244.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	91	rVB	219630	233702	16.38%	2.224%
2	1.535	147	154	169	rVB	170342	197911	13.87%	1.883%
3	2.063	308	318	335	rBV	278093	411446	28.83%	3.915%
4	2.561	470	473	476	rBV3	759	504	0.04%	0.005%
5	2.754	531	533	537	rBV3	439	292	0.02%	0.003%
6	2.825	553	555	558	rBV3	568	364	0.03%	0.003%
7	2.918	582	584	586	rBV2	353	144	0.01%	0.001%
8	2.950	593	594	595	rBV	278	72	0.01%	0.001%
9	3.024	614	617	621	rVB3	818	616	0.04%	0.006%
10	3.236	681	683	685	rBV2	633	391	0.03%	0.004%
11	3.262	690	691	694	rBV2	440	224	0.02%	0.002%
12	3.285	696	698	702	rBV	660	362	0.03%	0.003%
13	3.326	709	711	714	rBV	264	135	0.01%	0.001%
14	3.362	720	722	723	rBV	447	216	0.02%	0.002%
15	3.407	735	736	741	rBV4	398	277	0.02%	0.003%
16	3.458	746	752	754	rBV4	521	485	0.03%	0.005%
17	3.487	758	761	763	rBV	359	264	0.02%	0.003%
18	3.523	770	772	774	rBV2	414	178	0.01%	0.002%
19	3.535	774	776	777	rBV2	341	117	0.01%	0.001%
20	3.580	789	790	792	rBV	224	97	0.01%	0.001%
21	3.593	792	794	799	rVB3	771	610	0.04%	0.006%
22	3.622	799	803	807	rBV4	614	564	0.04%	0.005%
23	3.642	807	809	812	rVB2	391	236	0.02%	0.002%
24	3.661	812	815	818	rBV2	603	457	0.03%	0.004%
25	3.764	844	847	848	rBV2	411	201	0.01%	0.002%
26	3.796	848	857	896	rBV	100892	303753	21.29%	2.890%
27	4.256	985	1000	1030	rBV	232079	598887	41.97%	5.699%
28	4.696	1135	1137	1138	rBV	604	318	0.02%	0.003%
29	4.770	1158	1160	1163	rBV2	437	293	0.02%	0.003%
30	4.783	1163	1164	1167	rVV2	711	333	0.02%	0.003%
31	4.809	1170	1172	1176	rVB2	364	260	0.02%	0.002%
32	4.834	1176	1180	1182	rBV2	1024	719	0.05%	0.007%
33	4.899	1198	1200	1201	rBV2	399	150	0.01%	0.001%
34	4.963	1201	1220	1246	rBV2	535040	1426957	100.00%	13.578%
35	5.539	1386	1399	1437	rBV	413699	872742	61.16%	8.305%
36	5.995	1527	1541	1564	rBV	322071	684118	47.94%	6.510%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052623\
 Data File : VV031244.D
 Acq On : 26 May 2023 09:39
 Operator : SY/MD
 Sample : VV0526MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK345

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	6.262	1622	1624	1629	rVB3	734	600	0.04%	0.006%
38	6.285	1629	1631	1633	rBV2	1005	589	0.04%	0.006%
39	6.320	1640	1642	1643	rVB2	170	61	0.00%	0.001%
40	6.342	1643	1649	1651	rBV3	534	425	0.03%	0.004%
41	6.410	1667	1670	1672	rBV	589	450	0.03%	0.004%
42	6.468	1687	1688	1689	rBV	331	65	0.00%	0.001%
43	6.500	1693	1698	1703	rBV3	499	405	0.03%	0.004%
44	6.535	1706	1709	1711	rBV	515	291	0.02%	0.003%
45	6.561	1711	1717	1726	rBV8	1317	2001	0.14%	0.019%
46	6.664	1747	1749	1754	rVB4	617	399	0.03%	0.004%
47	6.686	1754	1756	1763	rBV4	737	711	0.05%	0.007%
48	6.719	1763	1766	1769	rBV3	379	241	0.02%	0.002%
49	6.731	1769	1770	1771	rBV	413	108	0.01%	0.001%
50	6.815	1792	1796	1797	rBV2	435	288	0.02%	0.003%
51	6.838	1800	1803	1805	rVB2	394	219	0.02%	0.002%
52	6.870	1810	1813	1815	rBV	372	212	0.01%	0.002%
53	6.918	1817	1828	1851	rBV	139735	265347	18.60%	2.525%
54	7.249	1918	1931	1962	rBV	527654	957955	67.13%	9.115%
55	7.558	2015	2027	2047	rBV	102397	190508	13.35%	1.813%
56	7.841	2111	2115	2117	rBV3	886	601	0.04%	0.006%
57	7.947	2146	2148	2150	rBV2	236	127	0.01%	0.001%
58	7.985	2157	2160	2164	rVB3	850	697	0.05%	0.007%
59	8.034	2164	2175	2216	rBV	317040	647997	45.41%	6.166%
60	8.403	2288	2290	2294	rBV3	764	473	0.03%	0.005%
61	8.702	2380	2383	2384	rBV	722	376	0.03%	0.004%
62	8.741	2392	2395	2396	rBV	350	189	0.01%	0.002%
63	8.789	2396	2410	2432	rBV	602784	1006904	70.56%	9.581%
64	9.024	2480	2483	2487	rBV5	895	915	0.06%	0.009%
65	9.124	2511	2514	2517	rBV3	733	618	0.04%	0.006%
66	9.188	2532	2534	2540	rVB3	1278	910	0.06%	0.009%
67	9.230	2545	2547	2550	rBV2	660	393	0.03%	0.004%
68	9.288	2562	2565	2573	rVB2	616	510	0.04%	0.005%
69	9.323	2573	2576	2583	rBV4	921	1054	0.07%	0.010%
70	9.352	2583	2585	2586	rBV	521	174	0.01%	0.002%
71	9.403	2599	2601	2605	rBV5	668	511	0.04%	0.005%
72	9.577	2653	2655	2658	rVB2	769	426	0.03%	0.004%
73	9.596	2658	2661	2663	rBV2	589	389	0.03%	0.004%
74	9.718	2696	2699	2704	rVB3	704	598	0.04%	0.006%
75	9.744	2704	2707	2709	rBV3	769	466	0.03%	0.004%
76	9.767	2711	2714	2716	rVB	688	381	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052623\
 Data File : VV031244.D
 Acq On : 26 May 2023 09:39
 Operator : SY/MD
 Sample : VV0526MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK345

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	9.812	2726	2728	2729	rBV	388	149	0.01%	0.001%
78	9.966	2772	2776	2777	rBV3	513	374	0.03%	0.004%
79	10.034	2795	2797	2799	rBV3	576	328	0.02%	0.003%
80	10.079	2809	2811	2813	rBV2	369	155	0.01%	0.001%
81	10.159	2824	2836	2861	rBV	451291	713858	50.03%	6.793%
82	10.468	2929	2932	2933	rBV2	607	356	0.02%	0.003%
83	10.609	2974	2976	2981	rBV2	518	420	0.03%	0.004%
84	10.712	3006	3008	3010	rBV	405	187	0.01%	0.002%
85	10.783	3029	3030	3033	rBV3	421	244	0.02%	0.002%
86	10.863	3049	3055	3057	rBV4	1602	1536	0.11%	0.015%
87	10.966	3084	3087	3091	rBV4	927	581	0.04%	0.006%
88	11.014	3100	3102	3108	rVB2	547	296	0.02%	0.003%
89	11.040	3108	3110	3113	rBV2	633	332	0.02%	0.003%
90	11.191	3146	3157	3179	rBV	593424	935876	65.59%	8.905%
91	11.497	3249	3252	3256	rVB3	512	399	0.03%	0.004%
92	11.567	3261	3274	3294	rBV	596682	944499	66.19%	8.987%
93	11.895	3374	3376	3378	rVB2	735	236	0.02%	0.002%
94	12.249	3482	3486	3489	rBV3	697	505	0.04%	0.005%
95	12.423	3538	3540	3542	rBV3	511	286	0.02%	0.003%
96	12.590	3586	3592	3603	rVB10	4907	8706	0.61%	0.083%
97	13.207	3776	3784	3794	rBV3	9487	14394	1.01%	0.137%
98	13.448	3850	3859	3872	rBV	26334	44190	3.10%	0.420%
99	13.693	3927	3935	3942	rBV3	11275	16722	1.17%	0.159%
100	14.365	4142	4144	4146	rBV3	1033	516	0.04%	0.005%




Sum of corrected areas: 10509124

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052623\
Data File : VV031244.D
Acq On : 26 May 2023 09:39
Operator : SY/MD
Sample : VV0526MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK345

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

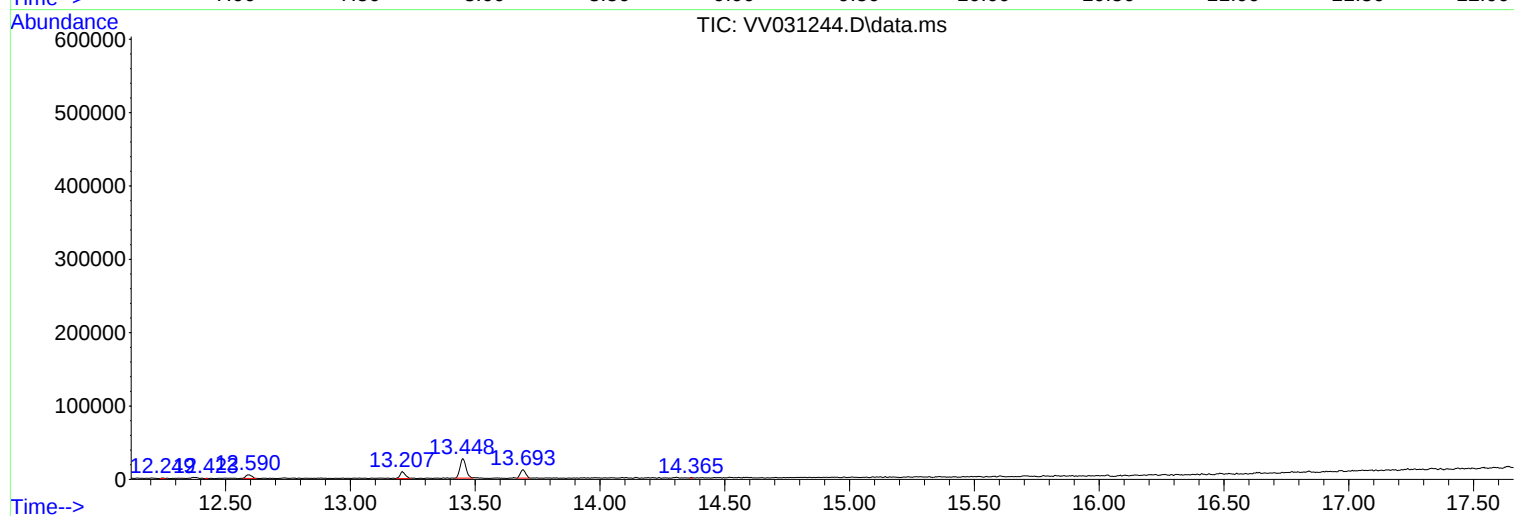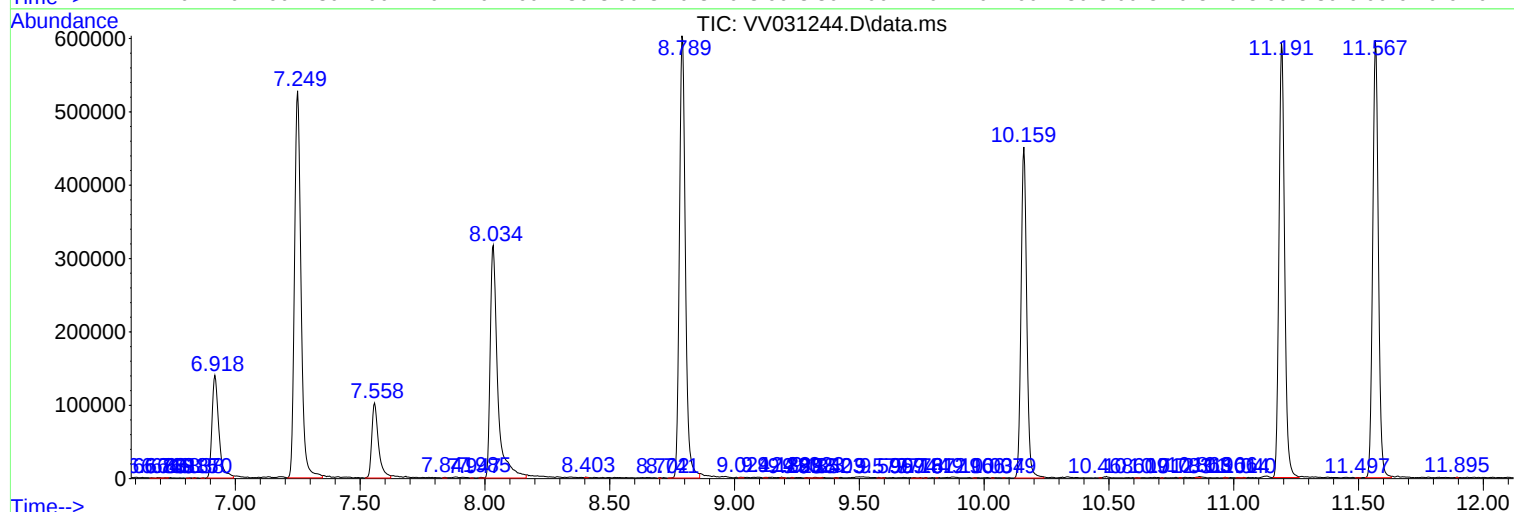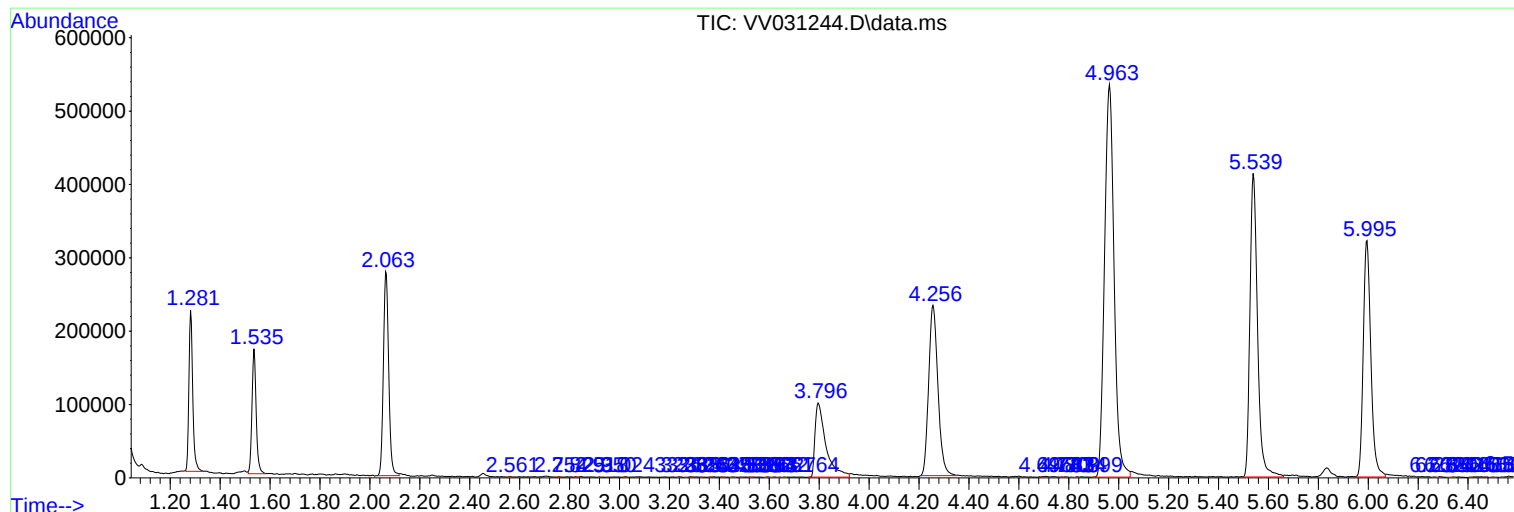

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052623\
Data File : VV031244.D
Acq On : 26 May 2023 09:39
Operator : SY/MD
Sample : VV0526MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK345

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052623\
Data File : VV031244.D
Acq On : 26 May 2023 09:39
Operator : SY/MD
Sample : VV0526MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK345

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc