

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052623\
 Data File : VV031247.D
 Acq On : 26 May 2023 12:26
 Operator : SY/MD
 Sample : VIBLK214
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK214

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	91	rVB	168198	178340	14.22%	1.976%
2	1.536	147	154	178	rVB	146985	173990	13.87%	1.927%
3	2.063	309	318	334	rVB	235975	342559	27.31%	3.795%
4	2.375	413	415	416	rBV	895	431	0.03%	0.005%
5	2.449	433	438	449	rVB3	5380	9401	0.75%	0.104%
6	2.600	480	485	486	rBV3	886	701	0.06%	0.008%
7	2.700	511	516	521	rBV4	1103	1176	0.09%	0.013%
8	2.773	537	539	540	rBV	403	197	0.02%	0.002%
9	2.825	552	555	558	rBV3	769	591	0.05%	0.007%
10	3.024	614	617	620	rBV3	631	488	0.04%	0.005%
11	3.124	646	648	652	rBV	424	309	0.02%	0.003%
12	3.191	665	669	670	rBV2	406	260	0.02%	0.003%
13	3.224	674	679	681	rBV3	586	478	0.04%	0.005%
14	3.275	693	695	700	rVB4	691	652	0.05%	0.007%
15	3.298	700	702	705	rVB2	472	190	0.02%	0.002%
16	3.365	720	723	725	rBV3	416	250	0.02%	0.003%
17	3.378	725	727	731	rVB	615	301	0.02%	0.003%
18	3.433	742	744	749	rVB2	513	430	0.03%	0.005%
19	3.465	749	754	758	rBV3	427	456	0.04%	0.005%
20	3.500	763	765	768	rBV3	567	367	0.03%	0.004%
21	3.564	783	785	789	rBV	468	384	0.03%	0.004%
22	3.654	810	813	817	rVB3	583	367	0.03%	0.004%
23	3.677	817	820	824	rVB4	448	366	0.03%	0.004%
24	3.706	825	829	834	rVB2	394	357	0.03%	0.004%
25	3.796	847	857	884	rBV	90720	269329	21.47%	2.983%
26	4.253	983	999	1029	rBV	207897	538758	42.95%	5.968%
27	4.545	1087	1090	1093	rBV3	354	258	0.02%	0.003%
28	4.664	1124	1127	1128	rBV	606	352	0.03%	0.004%
29	4.751	1150	1154	1156	rBV2	443	422	0.03%	0.005%
30	4.844	1180	1183	1185	rBV	355	220	0.02%	0.002%
31	4.960	1201	1219	1246	rBV3	462555	1254358	100.00%	13.895%
32	5.259	1308	1312	1316	rBV5	732	837	0.07%	0.009%
33	5.294	1321	1323	1325	rBV2	384	223	0.02%	0.002%
34	5.388	1349	1352	1355	rBV3	260	229	0.02%	0.003%
35	5.420	1361	1362	1366	rVB3	628	382	0.03%	0.004%
36	5.490	1380	1384	1385	rBV2	325	196	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW052623\
 Data File : VW031247.D
 Acq On : 26 May 2023 12:26
 Operator : SY/MD
 Sample : VIBLK214
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK214

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	5.539	1385	1399	1421	rBV	305060	633008	50.46%	7.012%
38	5.767	1469	1470	1472	rBV2	612	315	0.03%	0.003%
39	5.828	1480	1489	1505	rVB6	9710	21646	1.73%	0.240%
40	5.886	1505	1507	1509	rVB	691	248	0.02%	0.003%
41	5.902	1509	1512	1516	rVB2	512	381	0.03%	0.004%
42	5.992	1526	1540	1569	rBV	271967	566727	45.18%	6.278%
43	6.249	1618	1620	1625	rVB5	568	425	0.03%	0.005%
44	6.275	1625	1628	1630	rBV2	576	344	0.03%	0.004%
45	6.291	1630	1633	1636	rVB4	488	263	0.02%	0.003%
46	6.400	1665	1667	1669	rVB	630	178	0.01%	0.002%
47	6.478	1688	1691	1693	rBV2	485	266	0.02%	0.003%
48	6.535	1705	1709	1712	rBV2	632	498	0.04%	0.006%
49	6.558	1712	1716	1717	rBV2	893	601	0.05%	0.007%
50	6.629	1735	1738	1741	rBV3	672	395	0.03%	0.004%
51	6.770	1780	1782	1786	rVB2	760	377	0.03%	0.004%
52	6.793	1786	1789	1791	rBV2	484	340	0.03%	0.004%
53	6.915	1817	1827	1850	rBV	126346	239650	19.11%	2.655%
54	7.085	1877	1880	1882	rBV2	560	355	0.03%	0.004%
55	7.159	1900	1903	1907	rBV3	965	608	0.05%	0.007%
56	7.246	1918	1930	1954	rBV	432213	771772	61.53%	8.549%
57	7.558	2017	2027	2053	rBV	98519	185858	14.82%	2.059%
58	7.796	2099	2101	2104	rVB3	564	341	0.03%	0.004%
59	7.812	2104	2106	2108	rBV2	651	279	0.02%	0.003%
60	7.844	2113	2116	2118	rBV4	549	355	0.03%	0.004%
61	7.876	2122	2126	2131	rBV6	1164	1017	0.08%	0.011%
62	7.950	2147	2149	2151	rBV2	439	222	0.02%	0.002%
63	8.031	2164	2174	2214	rBV	302538	631760	50.37%	6.998%
64	8.567	2338	2341	2342	rBV2	541	284	0.02%	0.003%
65	8.635	2360	2362	2364	rBV	572	322	0.03%	0.004%
66	8.789	2393	2410	2437	rBV	539669	902045	71.91%	9.992%
67	9.236	2541	2549	2554	rBV6	807	1147	0.09%	0.013%
68	9.323	2574	2576	2578	rBV	529	293	0.02%	0.003%
69	9.368	2588	2590	2594	rBV2	423	301	0.02%	0.003%
70	9.445	2609	2614	2616	rBV4	622	555	0.04%	0.006%
71	9.468	2619	2621	2624	rBV2	538	316	0.03%	0.004%
72	9.493	2624	2629	2633	rBV6	782	788	0.06%	0.009%
73	9.532	2640	2641	2644	rVB2	966	429	0.03%	0.005%
74	9.551	2644	2647	2648	rBV	586	350	0.03%	0.004%
75	9.622	2667	2669	2671	rVB	484	171	0.01%	0.002%
76	9.638	2671	2674	2678	rBV2	420	325	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052623\
 Data File : VV031247.D
 Acq On : 26 May 2023 12:26
 Operator : SY/MD
 Sample : VIBLK214
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK214

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	9.744	2701	2707	2709	rBV4	759	520	0.04%	0.006%
78	9.847	2737	2739	2740	rBV2	433	191	0.02%	0.002%
79	9.931	2762	2765	2767	rBV	380	261	0.02%	0.003%
80	10.047	2796	2801	2807	rBV3	495	645	0.05%	0.007%
81	10.159	2825	2836	2859	rVB	418467	668082	53.26%	7.401%
82	10.294	2876	2878	2879	rBV2	522	192	0.02%	0.002%
83	10.329	2884	2889	2891	rBV5	1375	1320	0.11%	0.015%
84	10.461	2928	2930	2931	rBV	477	245	0.02%	0.003%
85	10.718	3008	3010	3011	rBV	514	182	0.01%	0.002%
86	10.844	3048	3049	3051	rBV	634	238	0.02%	0.003%
87	10.947	3079	3081	3084	rBV	551	311	0.02%	0.003%
88	10.995	3094	3096	3100	rVB2	549	245	0.02%	0.003%
89	11.024	3100	3105	3108	rBV3	429	487	0.04%	0.005%
90	11.191	3145	3157	3180	rBV	503996	791874	63.13%	8.772%
91	11.519	3255	3259	3261	rBV3	655	519	0.04%	0.006%
92	11.567	3261	3274	3294	rVV	505820	815308	65.00%	9.032%
93	12.005	3407	3410	3412	rBV3	689	392	0.03%	0.004%
94	12.136	3448	3451	3454	rBV2	415	267	0.02%	0.003%
95	12.268	3490	3492	3495	rBV3	536	255	0.02%	0.003%
96	12.329	3509	3511	3513	rBV	839	338	0.03%	0.004%
97	12.738	3636	3638	3640	rBV	566	277	0.02%	0.003%
98	13.111	3752	3754	3755	rBV	704	305	0.02%	0.003%
99	13.294	3809	3811	3814	rBV2	682	273	0.02%	0.003%
100	13.821	3974	3975	3978	rBV2	677	409	0.03%	0.005%




Sum of corrected areas: 9027296

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052623\
Data File : VV031247.D
Acq On : 26 May 2023 12:26
Operator : SY/MD
Sample : VIBLK214
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK214

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

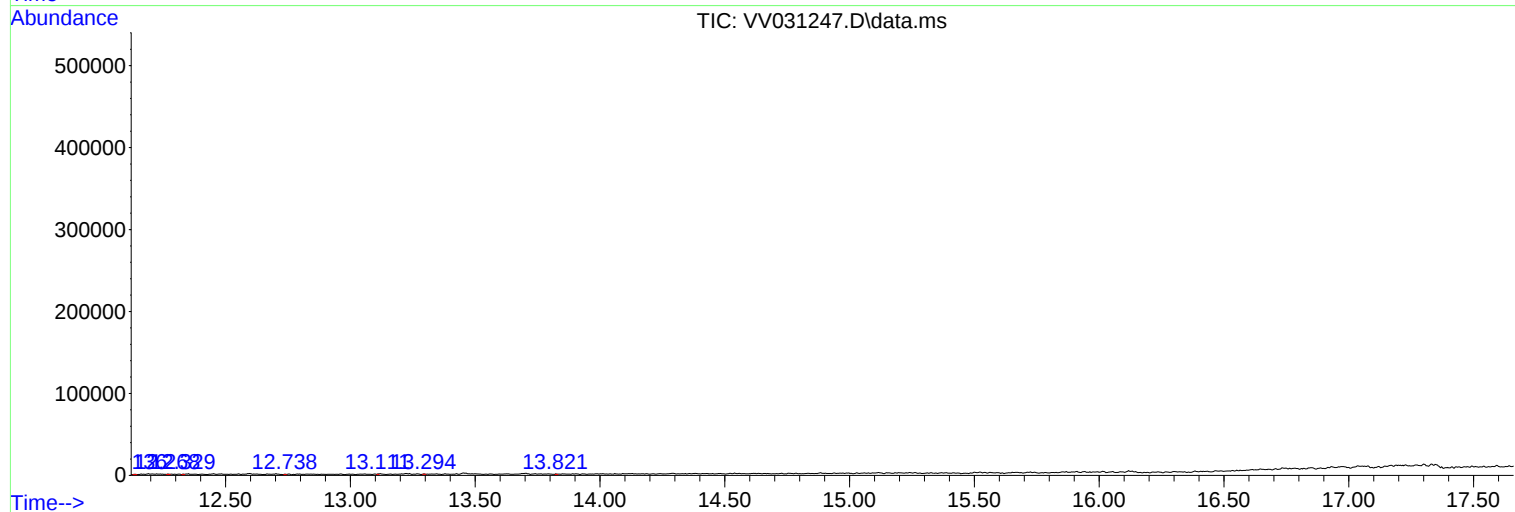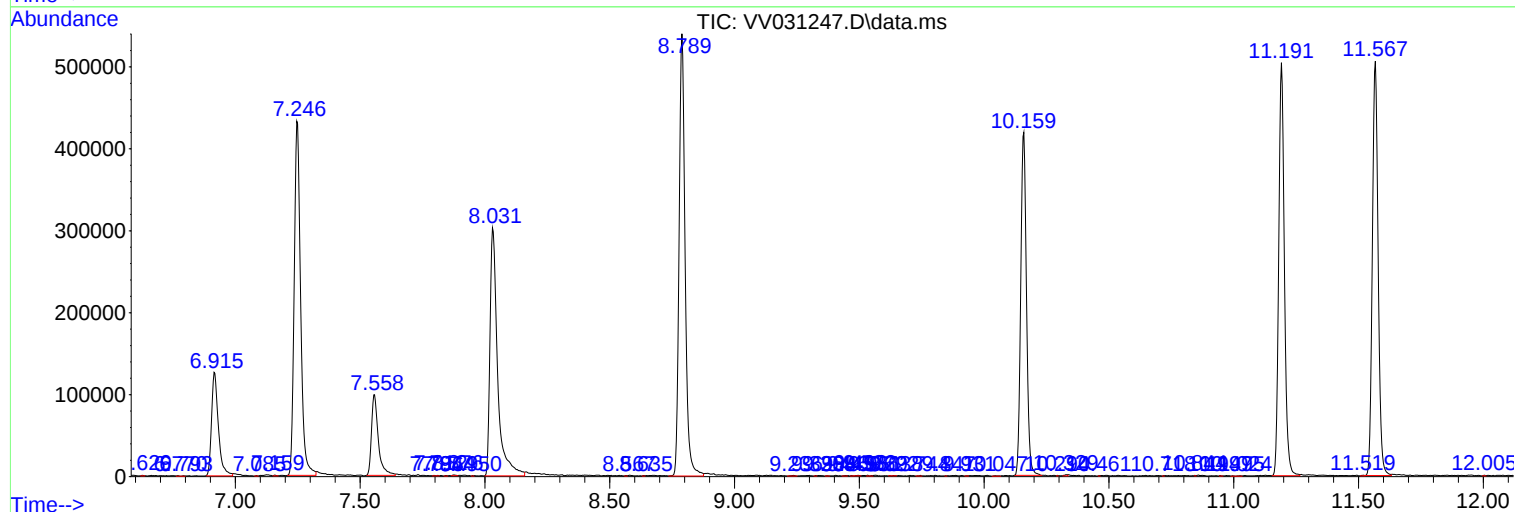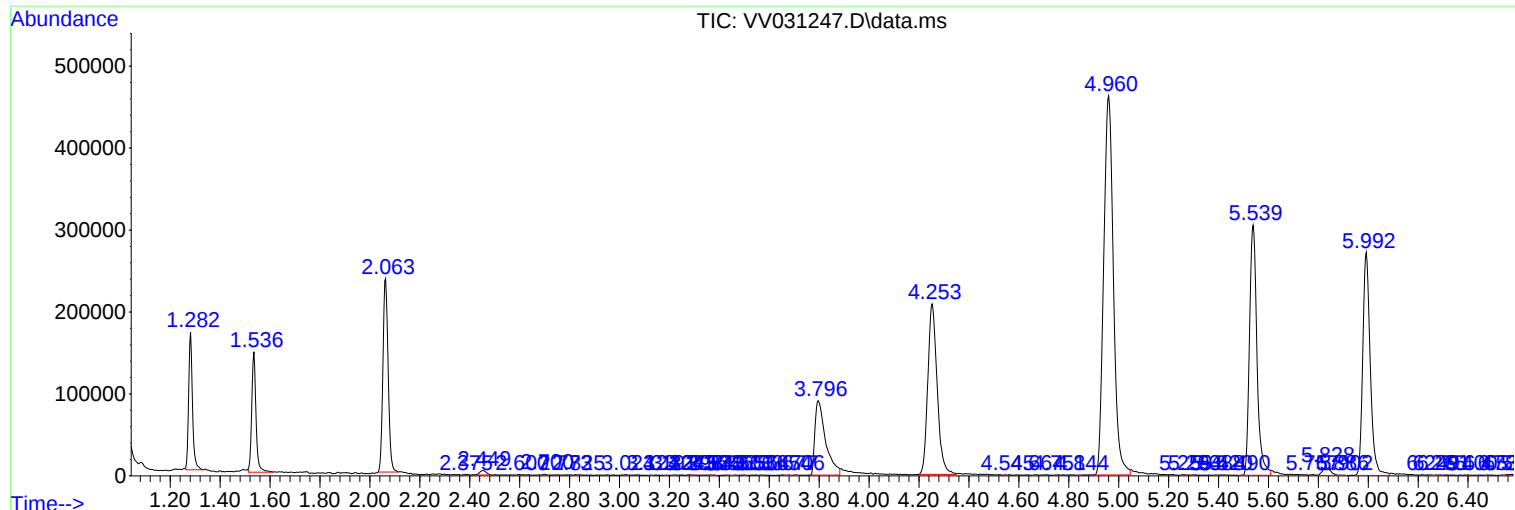

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052623\
Data File : VV031247.D
Acq On : 26 May 2023 12:26
Operator : SY/MD
Sample : VIBLK214
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK214

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052623\
Data File : VV031247.D
Acq On : 26 May 2023 12:26
Operator : SY/MD
Sample : VIBLK214
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK214

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------