


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052623\
Data File : VV031242.D
Acq On : 26 May 2023 08:38
Operator : SY/MD
Sample : BFB380
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB380

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Title : VOC Analysis
Last Update : Sat May 27 00:51:17 2023

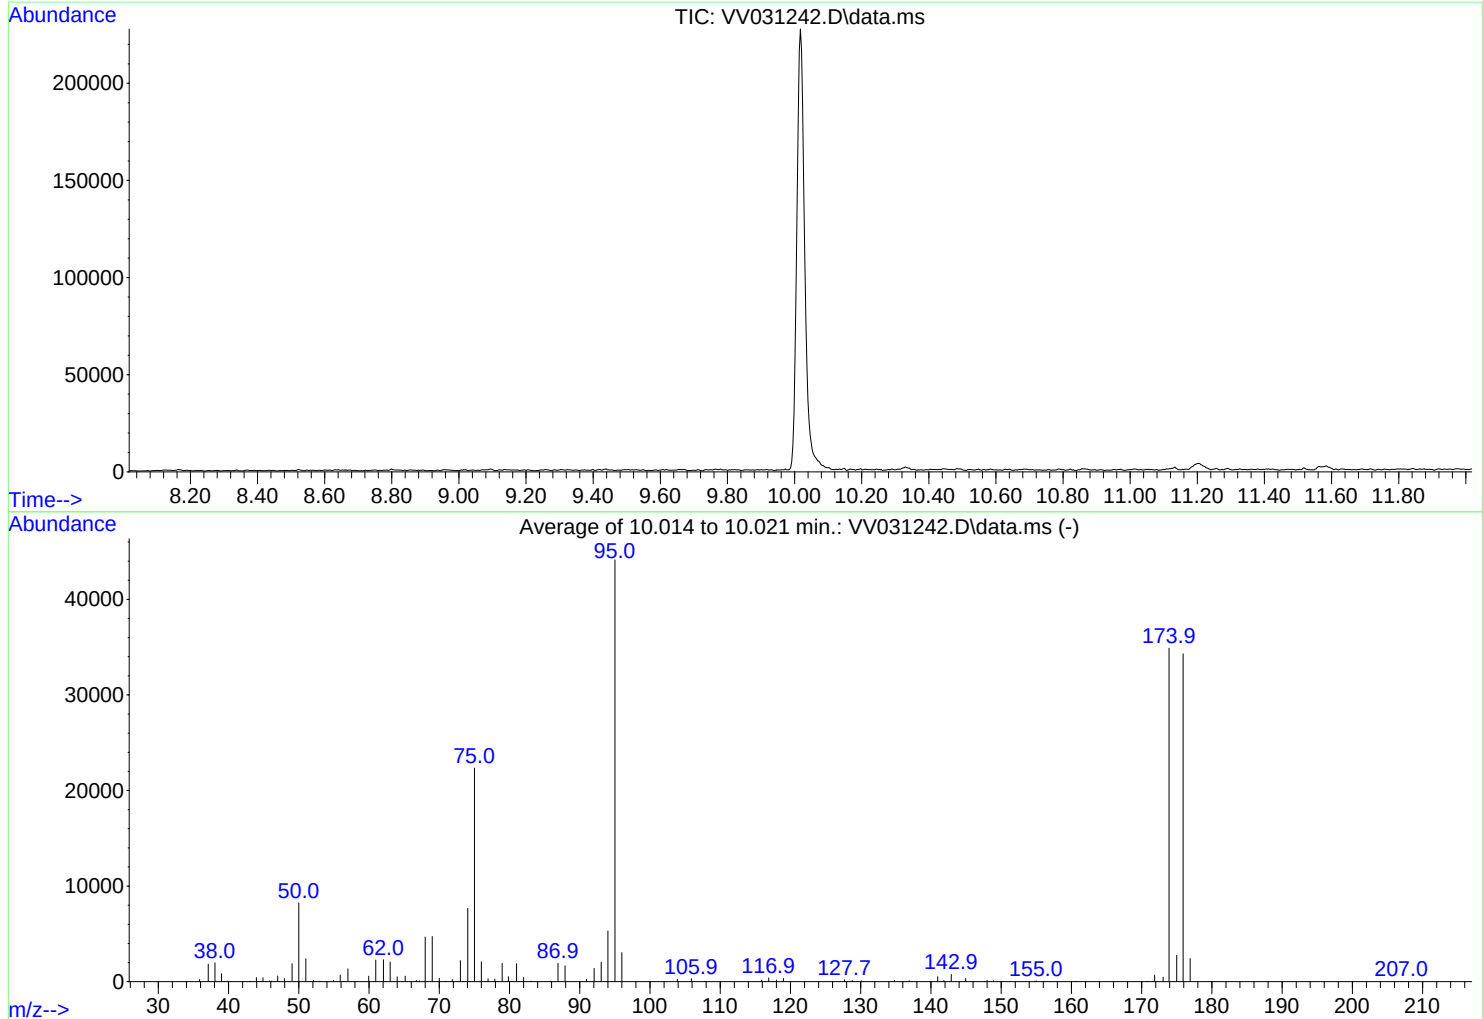

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2780

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	8231	PASS
75	95	30	80	50.6	22347	PASS
95	95	100	100	100.0	44136	PASS
96	95	5	9	6.9	3031	PASS
173	174	0.00	2	1.4	474	PASS
174	95	50	120	79.0	34885	PASS
175	174	5	9	7.9	2741	PASS
176	174	95	105	98.3	34309	PASS
177	176	5	10	7.0	2408	PASS

m/z	Abundance
35.90	146.0
37.80	122.0
39.90	385.0
43.90	407.0

Instrument :
MSVOA_V
ClientSampleId :
BFB380

m/z	Abundance
35.90	377.0
37.10	1778.0
38.10	2010.0
39.00	884.0
39.90	422.0
43.10	105.0
44.00	745.0
44.90	399.0
45.80	142.0
47.00	615.0
48.00	376.0
49.00	1907.0
50.00	8157.0
51.00	2398.0
52.10	150.0
55.00	160.0
55.90	748.0
57.00	1284.0
60.00	600.0
60.90	2214.0
62.00	2177.0
63.00	1987.0
64.00	491.0
65.20	449.0
66.80	130.0
68.00	4619.0
69.00	4566.0
70.00	352.0
70.90	109.0
71.80	225.0
73.00	2146.0
74.00	7902.0
75.00	21984.0
76.00	2198.0
77.00	317.0
78.00	255.0
78.90	1889.0
79.80	551.0
81.00	1944.0
82.00	415.0
83.10	140.0
85.80	132.0
86.90	1773.0
87.90	1697.0
90.90	217.0
92.10	1522.0
93.10	2018.0
94.00	5086.0
95.00	44048.0
96.00	2858.0
104.00	318.0
105.90	251.0
115.90	184.0
116.90	417.0
118.00	170.0
119.00	356.0
127.70	216.0
130.10	127.0
134.70	118.0
136.90	169.0
140.90	508.0
141.80	117.0
143.00	787.0
144.90	310.0
148.00	147.0
148.90	138.0
154.80	100.0
170.80	117.0
171.90	477.0
173.90	33736.0
175.00	2717.0
175.90	32984.0
176.90	2244.0
207.00	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB380

m/z	Abundance
35.90	360.0
37.10	1890.0
38.10	2059.0
39.00	864.0
39.90	478.0
44.00	873.0
44.90	433.0
45.90	122.0
47.00	589.0
48.00	297.0
49.00	1913.0
50.00	8510.0
51.00	2391.0
52.10	165.0
54.90	134.0
55.90	702.0
57.00	1372.0
59.90	597.0
61.00	2340.0
62.00	2425.0
63.00	2125.0
64.00	518.0
65.20	554.0
66.80	127.0
67.20	122.0
68.00	4825.0
69.00	4898.0
70.00	365.0
71.80	211.0
73.00	2274.0
74.00	7950.0
75.00	22992.0
76.00	2124.0
77.00	285.0
77.90	282.0
78.90	1993.0
79.90	537.0
81.00	1879.0
82.00	468.0
86.90	1981.0
87.90	1711.0
91.00	267.0
92.10	1399.0
93.10	2097.0
94.00	5516.0
95.00	45600.0
96.00	3177.0
103.90	238.0
105.90	315.0
115.90	167.0
116.90	397.0
118.00	163.0
119.00	343.0
127.70	192.0
128.80	166.0
130.10	128.0
134.80	122.0
136.90	130.0
140.90	533.0
141.90	141.0
142.90	775.0
144.90	338.0
148.00	149.0
148.90	137.0
155.00	111.0
160.70	110.0
171.80	719.0
173.10	704.0
173.90	36072.0
175.00	2858.0
175.90	35584.0
176.90	2533.0

Instrument :
MSVOA_V
ClientSampleId :
BFB380

m/z	Abundance
35.90	374.0
37.10	1805.0
38.00	1858.0
39.00	768.0
39.90	451.0
44.00	863.0
44.90	382.0
46.10	142.0
47.00	563.0
47.90	271.0
49.10	1791.0
50.00	8027.0
51.00	2385.0
52.10	120.0
53.00	133.0
54.90	121.0
55.90	628.0
57.00	1340.0
59.90	518.0
61.00	2215.0
62.10	2303.0
63.00	2080.0
64.00	479.0
65.10	685.0
66.70	110.0
67.20	148.0
68.00	4547.0
69.00	4721.0
70.00	356.0
71.90	230.0
73.00	2153.0
74.10	7141.0
75.00	22064.0
76.00	1900.0
76.90	298.0
77.80	272.0
79.00	1826.0
79.90	489.0
81.00	1799.0
82.00	440.0
86.90	2050.0
87.90	1583.0
91.00	295.0
92.00	1226.0
93.00	2013.0
94.00	5334.0
95.00	42760.0
96.00	3058.0
103.80	223.0
105.90	340.0
107.80	101.0
115.90	146.0
116.90	335.0
118.00	152.0
119.00	319.0
127.70	199.0
128.80	192.0
134.90	124.0
141.00	509.0
141.90	113.0
142.80	726.0
145.00	352.0
147.60	101.0
148.00	102.0
155.00	147.0
171.80	820.0
173.00	719.0
173.90	34848.0
175.00	2648.0
175.90	34360.0
176.90	2446.0
178.00	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB380