


Data Path : W:\HPCHEM1\MSVOA V\DATA\VV052718\
Data File : VV006082.D
Acq On : 27 May 2018 12:44
Operator : SY/MD
Sample : BFB63
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : W:\HPCHEM1\MSVOA_V\METHOD\SOMVLM052718WMA.M
Title : VOC Analysis
Last Update : Mon May 28 00:47:58 2018

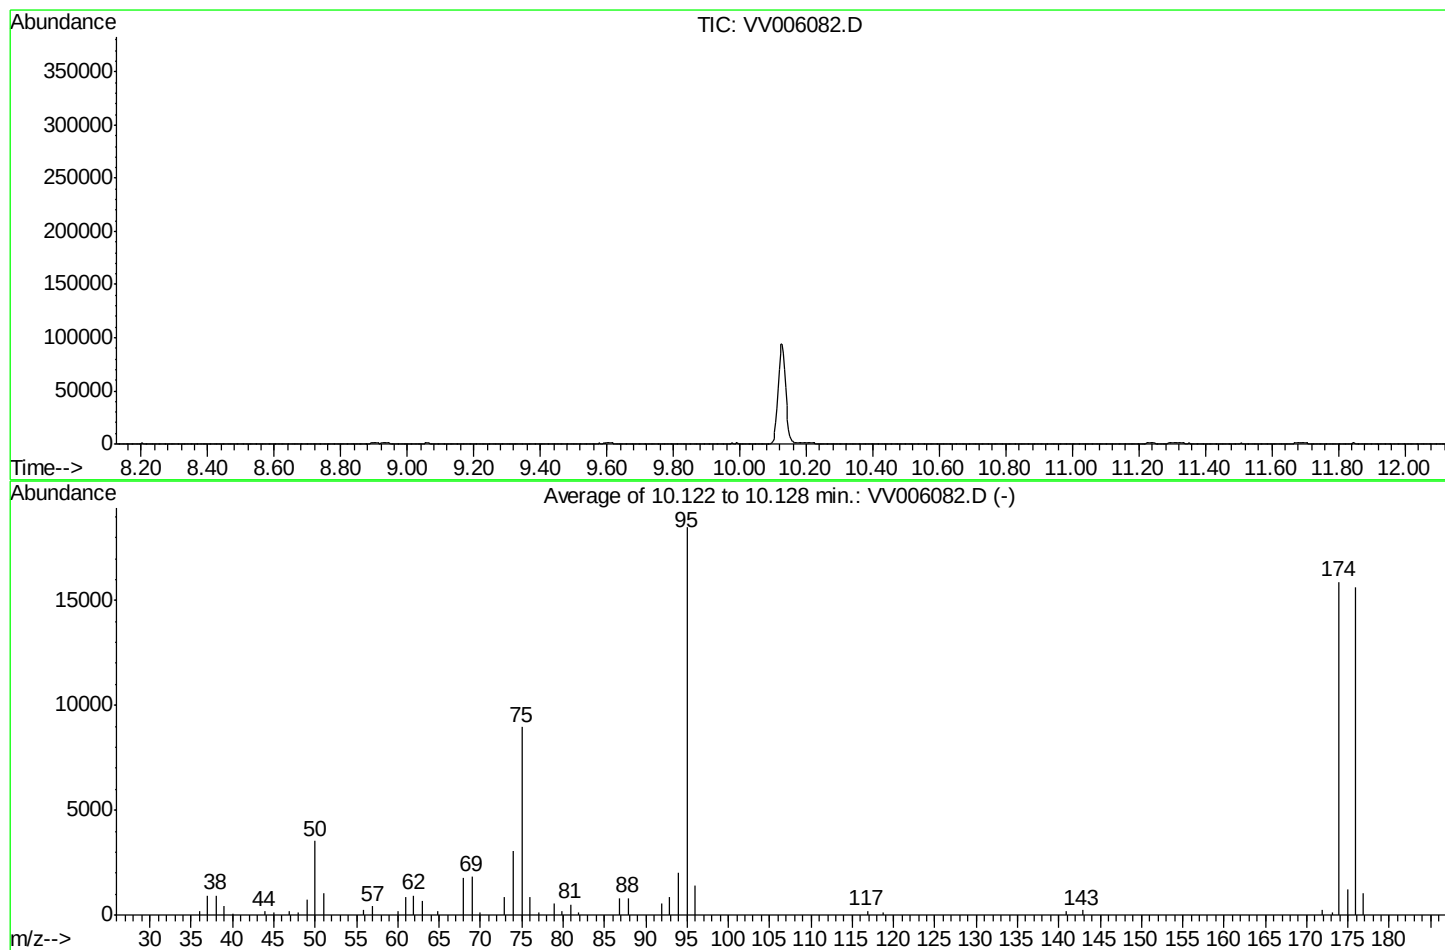

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2861

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	3537	PASS
75	95	30	80	48.5	8960	PASS
95	95	100	100	100.0	18490	PASS
96	95	5	9	7.7	1416	PASS
173	174	0.00	2	0.8	122	PASS
174	95	50	120	85.9	15878	PASS
175	174	5	9	7.7	1222	PASS
176	174	95	101	98.4	15620	PASS
177	176	5	9	6.7	1052	PASS

Scan 2861 (10.089 min): VV006082.D
BFB63

m/z	Abundance
43.80	353.0

Scan 2871 (10.122 min): VV006082.D
BFB63

m/z	Abundance
36.00	188.0
37.00	874.0
38.00	844.0
39.00	390.0
40.00	131.0
43.90	492.0
45.00	144.0
46.90	201.0
48.00	124.0
49.00	723.0
50.00	3314.0
51.00	1023.0
55.90	286.0
57.00	441.0
59.90	174.0
61.00	838.0
61.90	883.0
63.00	635.0
64.90	203.0
68.00	1688.0
69.00	1779.0
69.90	141.0
73.00	807.0
74.00	2938.0
75.00	8470.0
76.00	783.0
77.10	107.0
78.90	512.0
79.90	173.0
80.90	488.0
81.80	112.0
86.90	861.0
87.90	787.0
91.90	469.0
92.90	828.0
94.00	1763.0
95.00	17536.0
96.00	1300.0
116.80	172.0
118.80	115.0
141.00	130.0
142.80	200.0
171.90	190.0
173.00	179.0
173.90	14604.0
174.90	1145.0
175.90	14367.0
176.90	969.0

Scan 2872 (10.125 min): VV006082.D
BFB63

m/z	Abundance
36.00	188.0
37.00	950.0
38.00	993.0
38.90	422.0
40.00	110.0
43.90	541.0
45.00	136.0
46.90	189.0
47.90	124.0
49.00	768.0
50.00	3680.0
51.00	1081.0
55.90	258.0
57.00	426.0
60.00	190.0
61.00	906.0
61.90	942.0
63.00	690.0
64.90	220.0
67.90	1784.0
69.00	1882.0
69.90	140.0
73.00	880.0
74.00	3191.0
75.00	9270.0
76.00	888.0
77.00	122.0
78.90	569.0
79.90	195.0
80.90	509.0
81.80	122.0
86.90	827.0
87.90	850.0
91.90	579.0
92.90	877.0
94.00	2102.0
95.00	19064.0
96.00	1493.0
116.80	207.0
118.80	131.0
140.90	173.0
142.80	248.0
171.90	253.0
173.10	189.0
173.90	16400.0
174.90	1261.0
175.90	16129.0
176.90	1103.0

Scan 2873 (10.128 min): VV006082.D
BFB63

m/z	Abundance
35.90	183.0
37.00	957.0
38.00	954.0
38.90	400.0
43.90	557.0
44.90	125.0
46.90	175.0
47.90	114.0
49.00	729.0
50.00	3619.0
51.00	1066.0
55.90	245.0
56.90	414.0
60.00	208.0
61.00	861.0
61.90	940.0
63.00	729.0
64.90	199.0
68.00	1776.0
69.00	1802.0
70.00	133.0
72.90	877.0
74.00	3124.0
75.00	9141.0
76.00	881.0
77.00	140.0
78.90	615.0
79.90	204.0
80.90	490.0
81.90	135.0
86.90	776.0
87.90	843.0
91.90	595.0
92.90	864.0
94.00	2241.0
95.00	18872.0
96.00	1456.0
116.80	210.0
118.80	124.0
140.90	189.0
142.90	273.0
171.90	248.0
173.90	16632.0
174.90	1261.0
175.90	16364.0
176.90	1086.0