

Quantitation Report (QT Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052720\
 Data File : VV016222.D
 Acq On : 27 May 2020 12:49
 Operator : SY/MD
 Sample : L2754-10
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sample ID :
 GAX98

Manual Integrations
 APPROVED

Quant Time: May 28 02:47:41 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR052620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 28 01:17:22 2020
 Response via : Initial Calibration

MMDadoda
 5/29/2020 4:11:41 PM

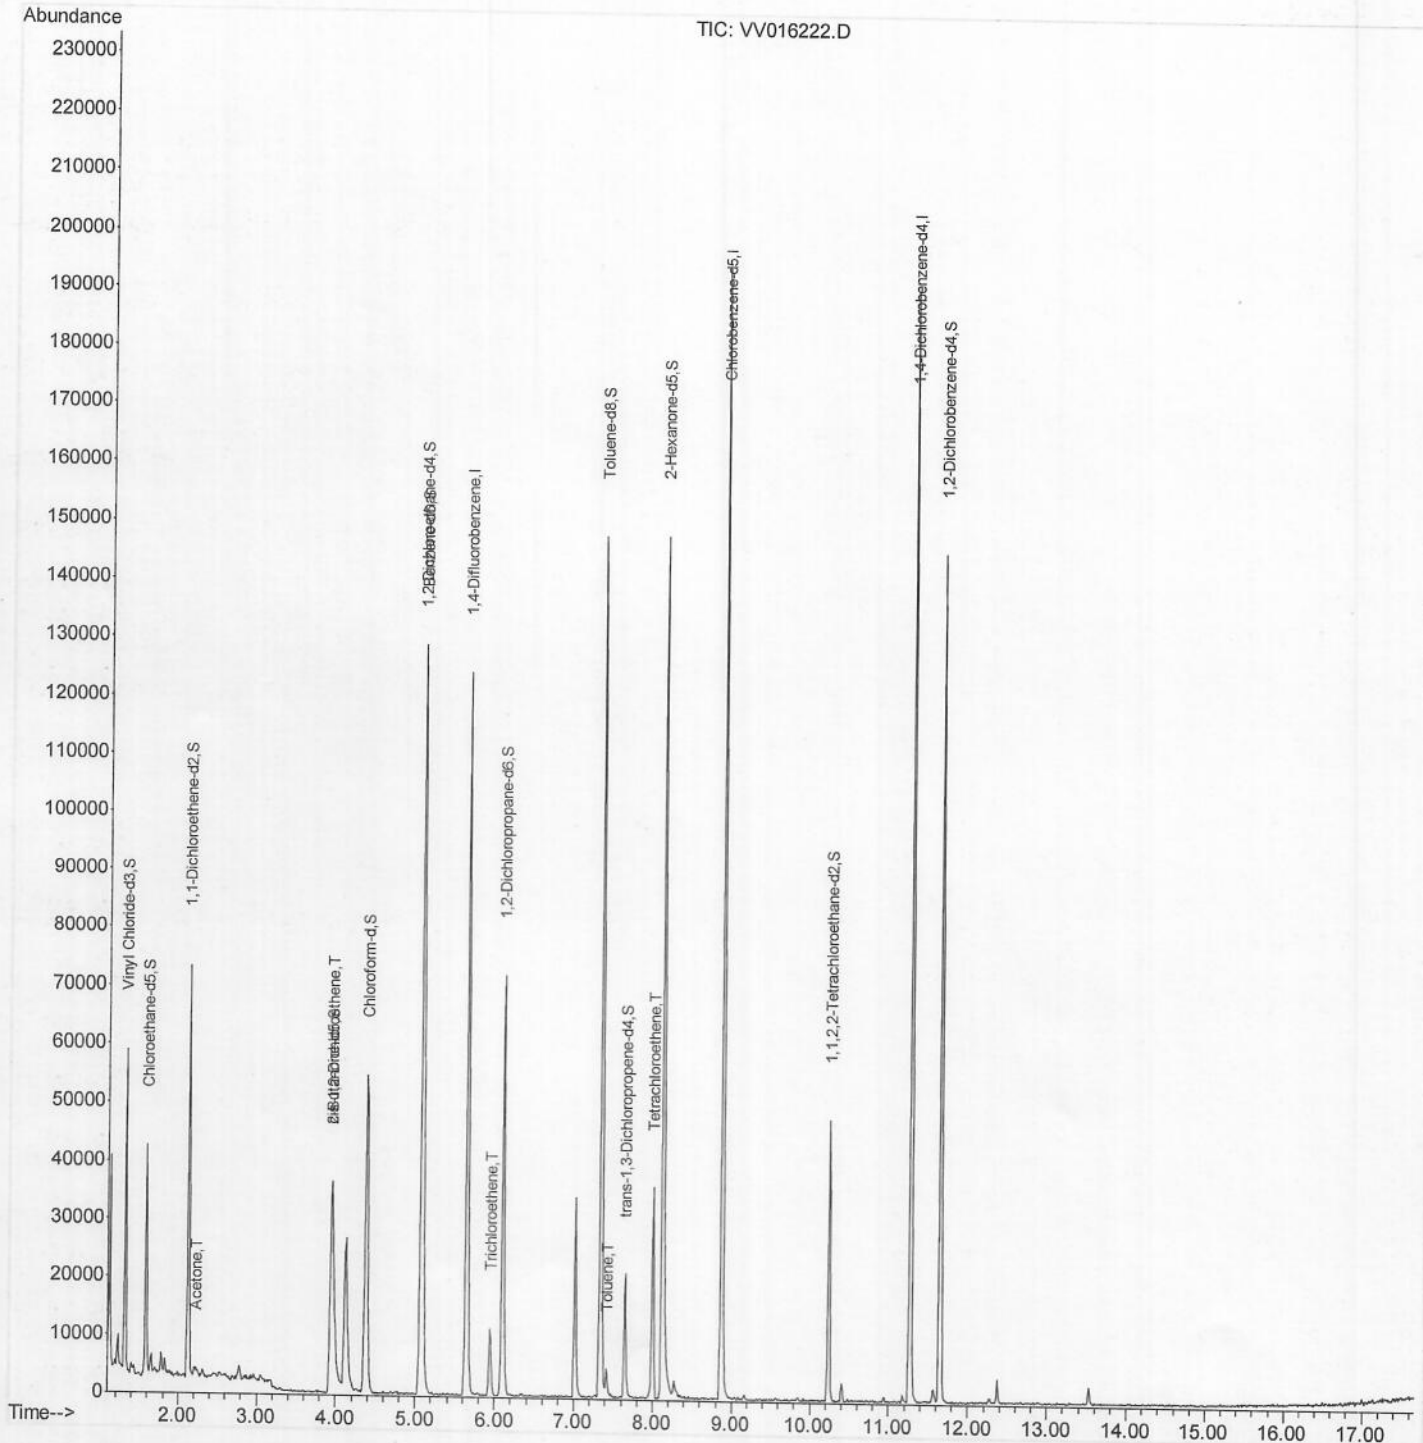

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052720\
Data File : VV016222.D
Acq On : 27 May 2020 12:49
Operator : SY/MD
Sample : L2754-10
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1




Instrument :
MSVOA_V
ClientSampleId :
GAX98

Manual Integrations
APPROVED

MMDadoda

5/29/2020 4:11:41 PM

Quant Time: May 28 01:20:40 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR052620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu May 28 01:17:22 2020
Response via : Initial Calibration

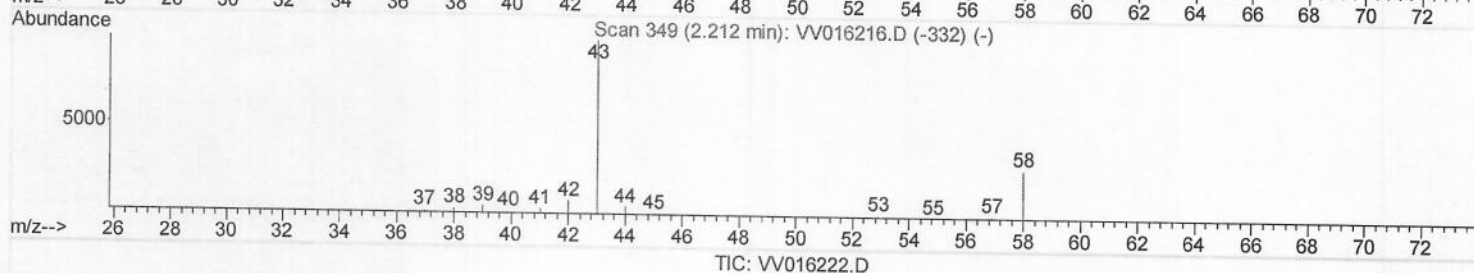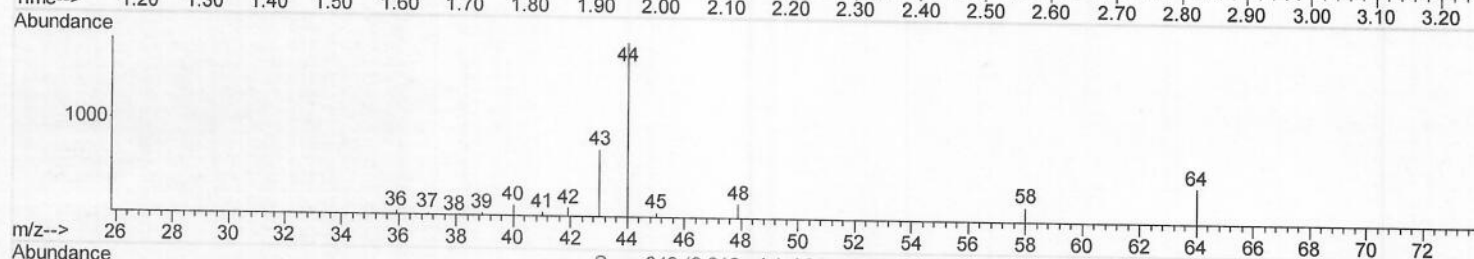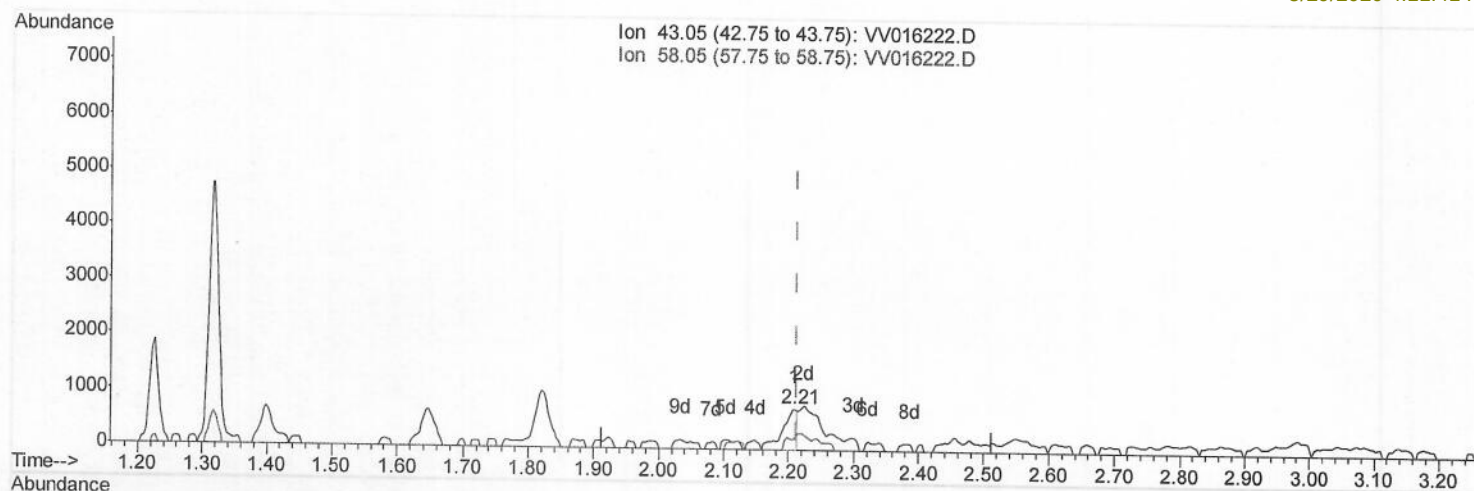

(13) Acetone (T)

2.209min (-0.003) 1.21ug/L

response 1171

Ion	Exp%	Act%
43.05	100	100
58.05	24.40	13.49
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052720\
 Data File : VV016222.D
 Acq On : 27 May 2020 12:49
 Operator : SY/MD
 Sample : L2754-10
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAX98

Manual Integrations
 APPROVED

Quant Time: May 28 01:20:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR052620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 28 01:17:22 2020
 Response via : Initial Calibration

MMDadoda
 5/29/2020 4:11:41 PM

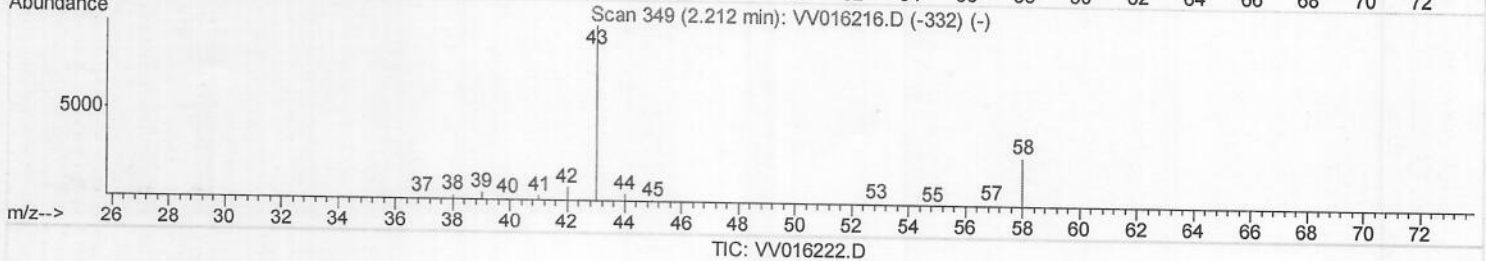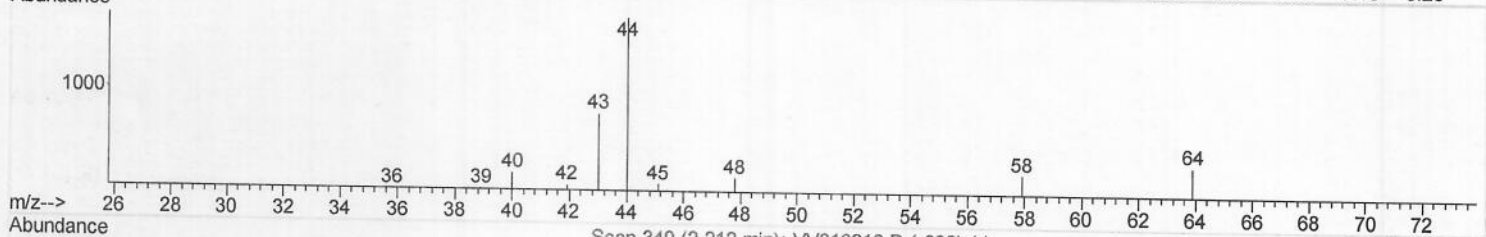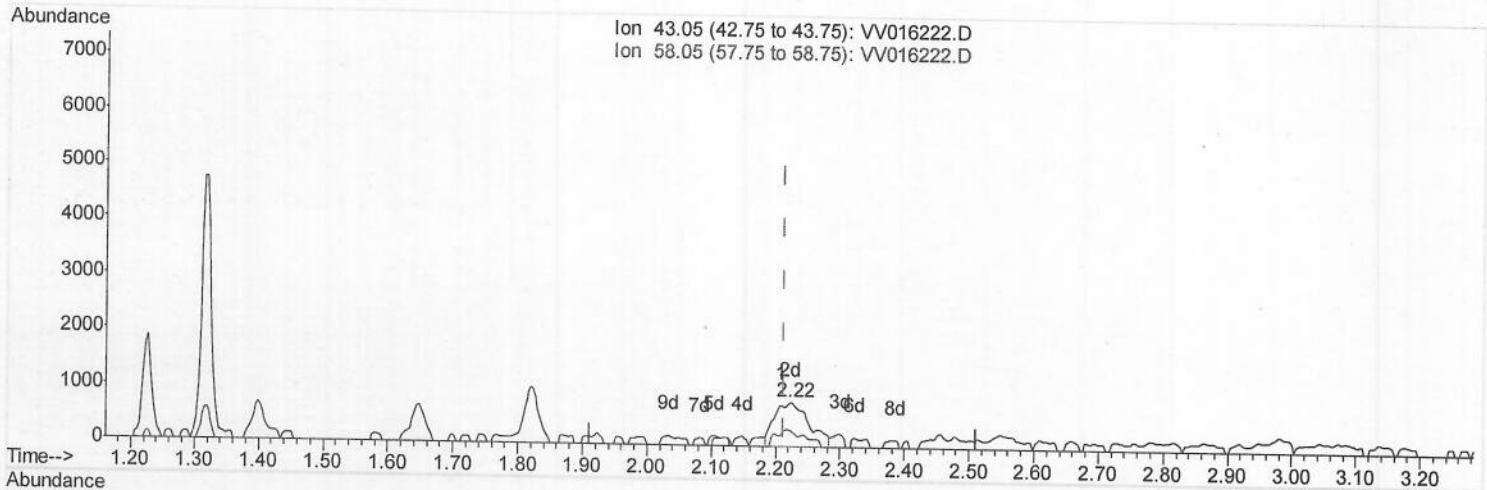

(13) Acetone (T)

2.222min (+0.010) 3.08ug/L m

response 2983

Ion	Exp%	Act%
43.05	100	100
58.05	24.40	5.30
0.00	0.00	0.00
0.00	0.00	0.00

M.D
 05/29/20

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052720\
 Data File : VV016222.D
 Acq On : 27 May 2020 12:49
 Operator : SY/MD
 Sample : L2754-10
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 GAX98

Manual Integrations
 APPROVED

MMDadoda

5/29/2020 4:11:41 PM

Quant Time: May 28 02:47:41 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR052620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 28 01:17:22 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	98198	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	95330	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	43754	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.32	65	26602	4.22	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	84.40%		
7) Chloroethane-d5	1.58	69	24435	4.41	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	88.20%		
11) 1,1-Dichloroethene-d2	2.13	63	38011	3.21	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	64.20%		
20) 2-Butanone-d5	3.95	46	69871	44.66	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	89.32%		
24) Chloroform-d	4.38	84	54273	4.32	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	86.40%		
26) 1,2-Dichloroethane-d4	5.06	65	29508	4.44	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	88.80%		
32) Benzene-d6	5.08	84	105563	4.47	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	89.40%		
36) 1,2-Dichloropropane-d6	6.10	67	32566	4.46	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	89.20%		
41) Toluene-d8	7.34	98	93281	4.14	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	82.80%		
45) trans-1,3-Dichloropropene-	7.65	79	11097	4.08	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	81.60%		
48) 2-Hexanone-d5	8.12	63	51096	40.91	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	81.82%		
59) 1,1,2,2-Tetrachloroethane-	10.24	84	22397	4.15	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	83.00%		
65) 1,2-Dichlorobenzene-d4	11.65	152	32842	4.49	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	89.80%		
Target Compounds						
13) Acetone	2.22	43	2983m	3.080	ug/L	Ovalue
22) cis-1,2-Dichloroethene	3.94	96	2493	0.333	ug/L	98
34) Trichloroethene	5.94	95	4247	0.594	ug/L	94
42) Toluene	7.42	91	3381	0.113	ug/L	94
49) Tetrachloroethene	8.00	164	7381	1.439	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

M.D
 05/29/20