

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052720\
 Data File : VV016243.D
 Acq On : 27 May 2020 21:45
 Operator : SY/MD
 Sample : VV0527WBL02
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK40

Quant Time: May 28 06:42:20 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR052620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 28 06:30:54 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	90764	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	88967	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	39554	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	26694	4.58	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.60%
7) Chloroethane-d5	1.58	69	24943	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.40%
11) 1,1-Dichloroethene-d2	2.13	63	38332	3.50	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.00%
20) 2-Butanone-d5	3.94	46	72993	50.48	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.96%
24) Chloroform-d	4.38	84	54497	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
26) 1,2-Dichloroethane-d4	5.06	65	29445	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.80%
32) Benzene-d6	5.08	84	104061	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
36) 1,2-Dichloropropane-d6	6.10	67	32710	4.80	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.00%
41) Toluene-d8	7.34	98	91140	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.80%
45) trans-1,3-Dichloropropene-	7.65	79	9900	3.90	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.00%
48) 2-Hexanone-d5	8.12	63	49580	42.54	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.08%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	22155	4.40	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.00%
65) 1,2-Dichlorobenzene-d4	11.65	152	32380	4.90	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.00%


Target Compounds					Ovalue
16) Methylene chloride	2.53	84	2947	0.480 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052720\
Data File : VV016243.D
Acq On : 27 May 2020 21:45
Operator : SY/MD
Sample : VV0527WBL02
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK40

Quant Time: May 28 06:42:20 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR052620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu May 28 06:30:54 2020
Response via : Initial Calibration

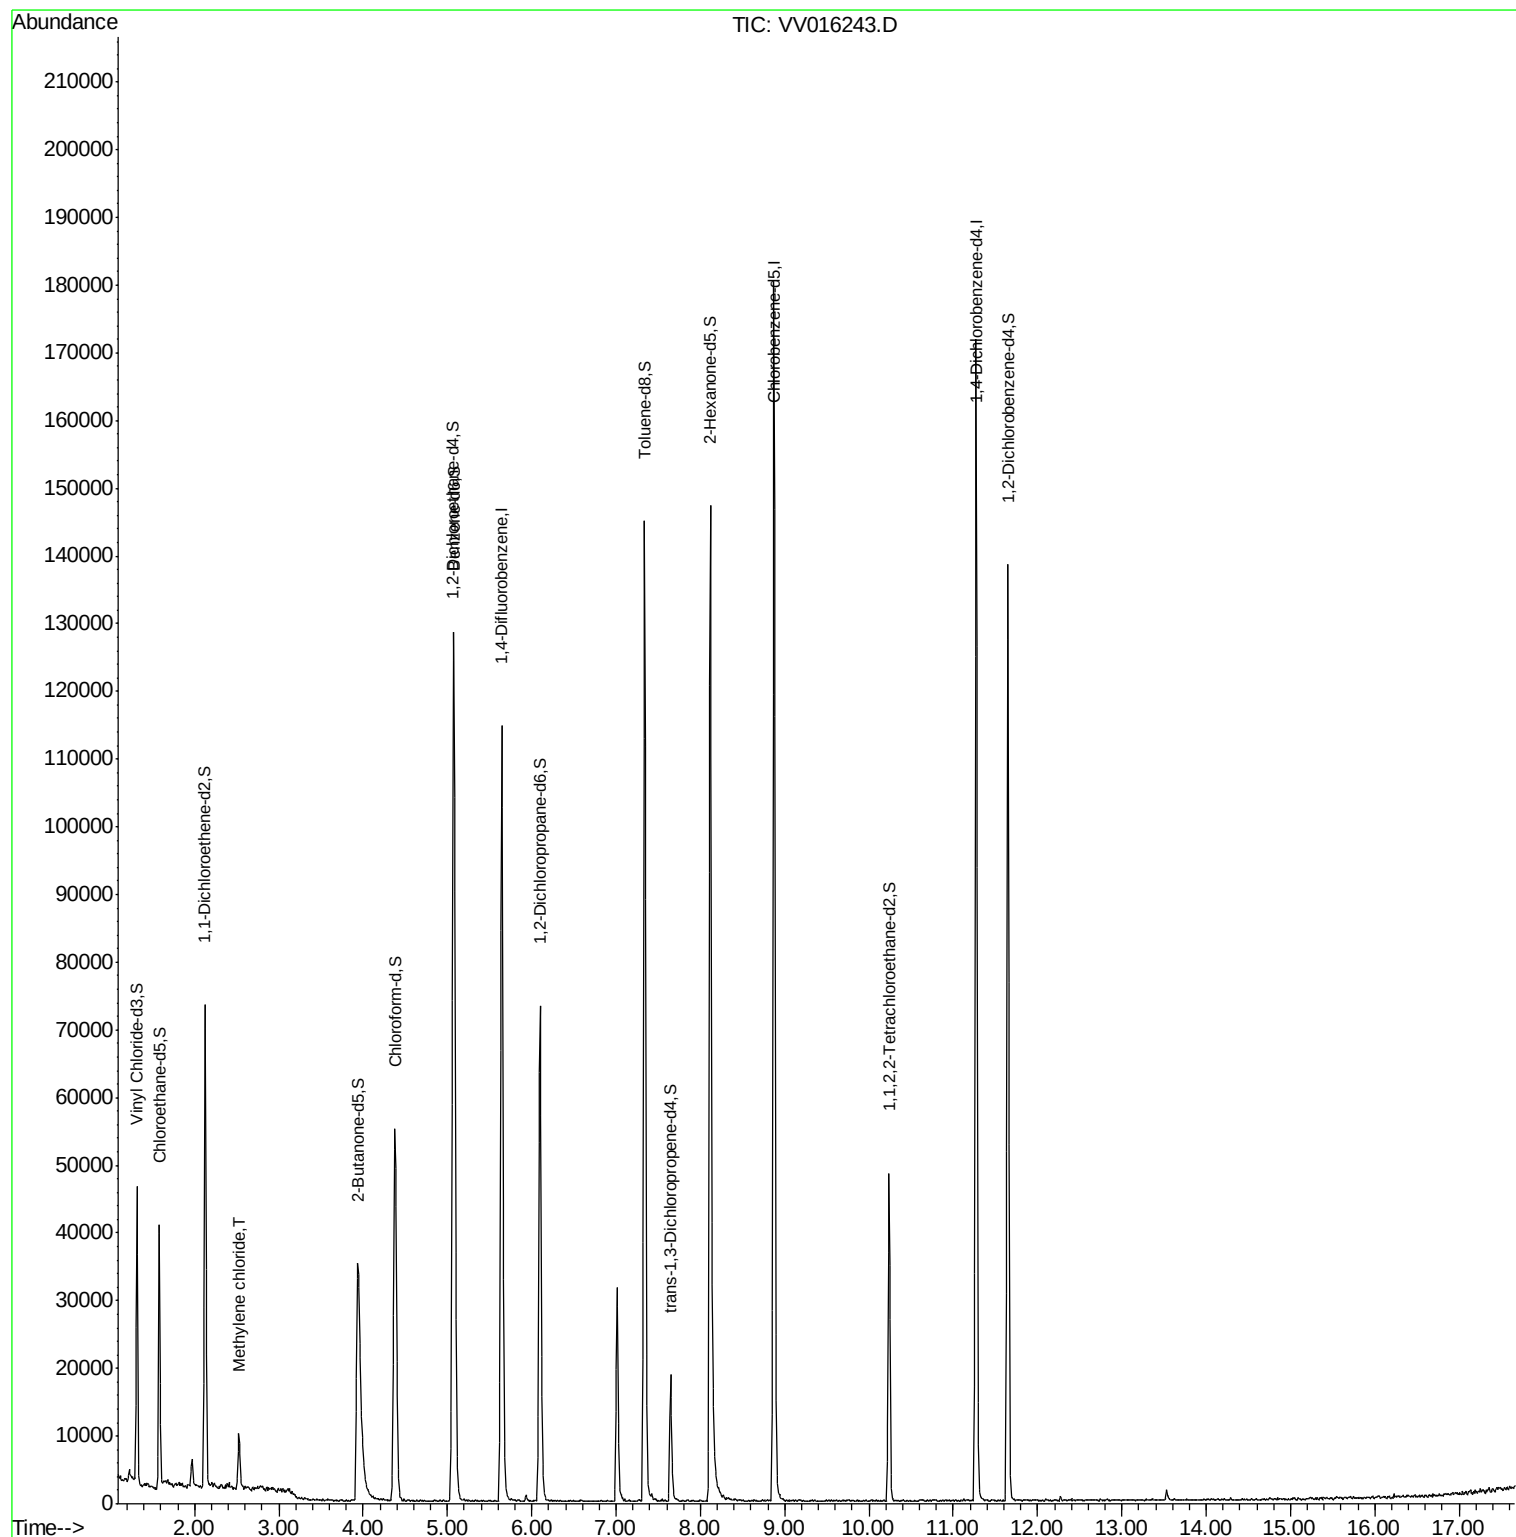

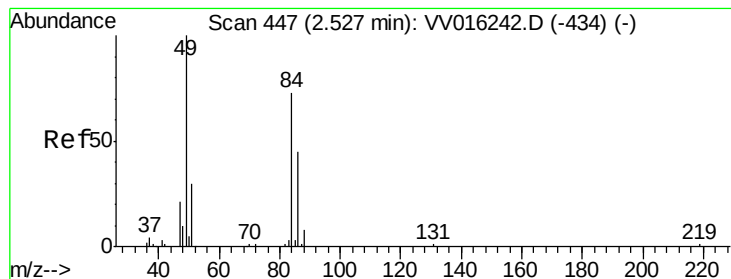

#16
Methylene chloride
Concen: 0.480 ug/L
RT: 2.53 min Scan# 447
Delta R.T. -0.00 min
Lab File: VV016243.D
Acq: 27 May 2020 21:45

Instrument :
MSVOA_V
ClientSampleId :
VBLK40

Tot Ion	Ratio	Lower	Upper
84	100		
86	73.0	44.9	83.5
49	141.9	96.7	179.7

