


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV052720\
 Data File : VV016215.D
 Acq On : 27 May 2020 09:30
 Operator : SY/MD
 Sample : BFB32
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB32

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR052620WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu May 28 06:30:54 2020

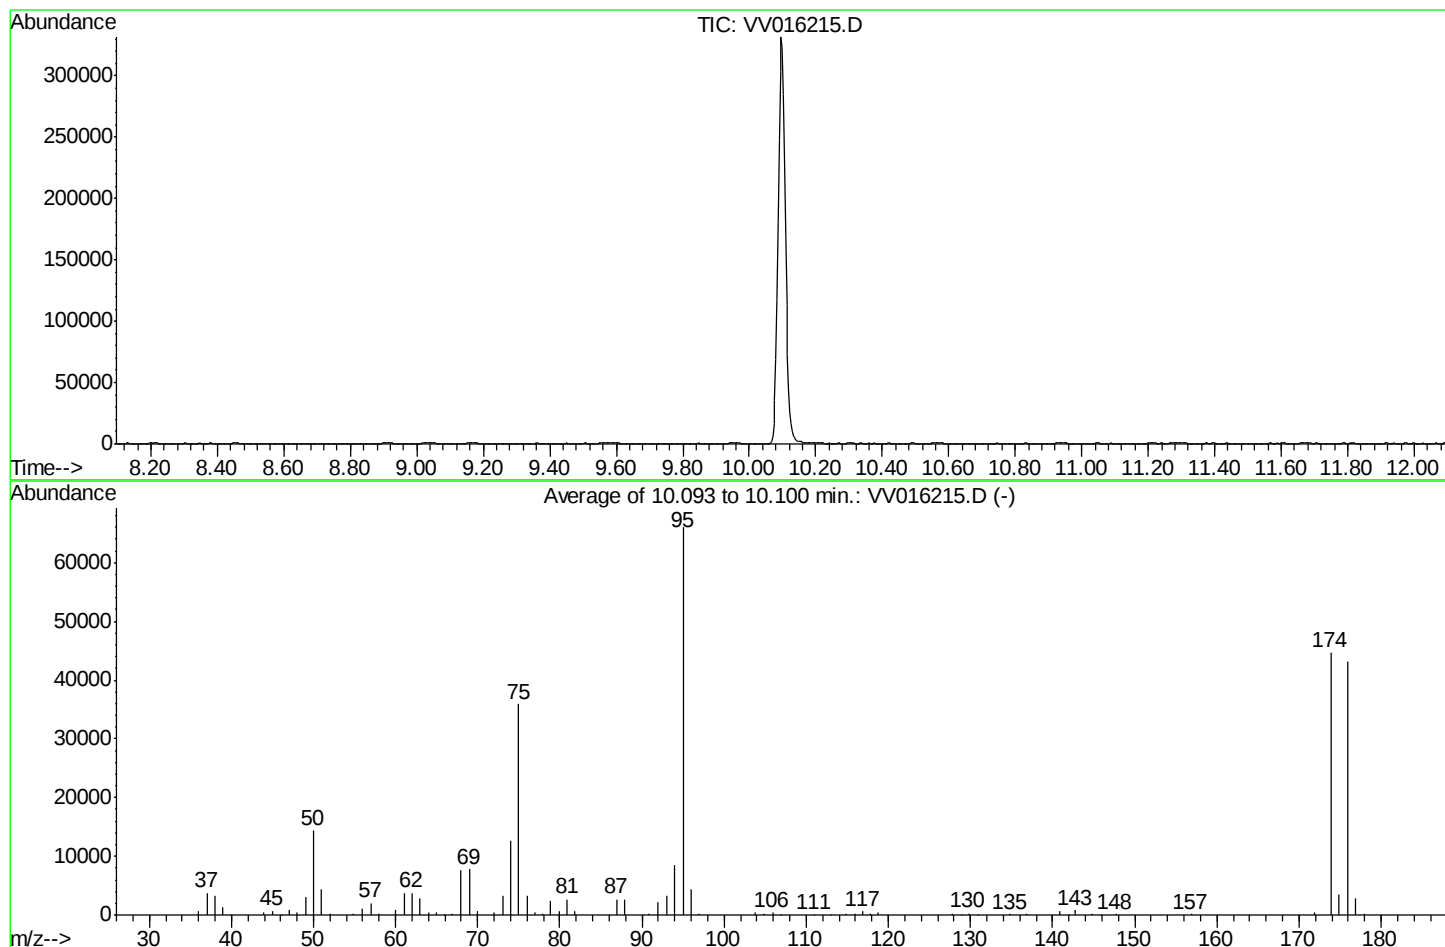

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	14331	PASS
75	95	30	80	54.4	35901	PASS
95	95	100	100	100.0	66018	PASS
96	95	5	9	6.5	4295	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.7	44685	PASS
175	174	5	9	7.8	3507	PASS
176	174	95	101	96.4	43088	PASS
177	176	5	9	6.7	2899	PASS

m/z	Abundance
36.00	641.0
37.00	3557.0
38.00	3130.0
39.00	1435.0
39.90	276.0
43.90	699.0
44.90	695.0
47.00	774.0
47.90	406.0
49.00	2887.0
50.00	13840.0
51.00	4336.0
52.00	195.0
54.90	257.0
56.00	949.0
57.00	1931.0
57.90	136.0
59.90	746.0
61.00	3544.0
62.00	3581.0
63.00	2671.0
64.10	359.0
65.00	339.0
65.90	100.0
66.90	243.0
68.00	7248.0
69.00	7587.0
70.00	550.0
71.90	428.0
73.00	3309.0
74.00	12103.0
75.00	34736.0
76.00	3244.0
77.00	436.0
77.90	269.0
78.90	2382.0
79.90	695.0
80.90	2736.0
81.90	674.0
86.90	2637.0
87.90	2303.0
90.90	299.0
92.00	2085.0
93.00	2979.0
94.00	8097.0
95.00	63312.0
96.00	4243.0
96.90	137.0
103.80	334.0
104.90	135.0
105.90	357.0
106.90	114.0
111.00	102.0
112.90	118.0
114.90	111.0
115.90	261.0
116.90	504.0
117.80	274.0
118.80	474.0
127.70	232.0
128.80	116.0
129.80	217.0
134.80	167.0
136.80	114.0
140.80	714.0
142.80	763.0
144.80	154.0
147.70	155.0
156.90	114.0
171.90	507.0
173.90	41344.0
174.90	3382.0
175.90	39360.0
176.90	2690.0
177.90	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

m/z	Abundance
36.00	621.0
37.00	3958.0
38.00	3498.0
39.00	1421.0
39.90	270.0
44.00	776.0
45.00	730.0
46.20	139.0
47.00	954.0
47.90	370.0
49.00	3142.0
50.00	14879.0
51.00	4640.0
52.00	213.0
54.90	254.0
56.00	1130.0
57.00	2127.0
57.90	137.0
59.90	809.0
61.00	3805.0
62.00	3840.0
63.00	2943.0
64.00	362.0
65.00	353.0
65.90	111.0
66.90	215.0
68.00	7870.0
69.00	8180.0
70.00	642.0
71.90	496.0
73.00	3388.0
74.00	13154.0
75.00	37296.0
76.00	3474.0
76.90	469.0
77.90	256.0
78.90	2533.0
79.90	763.0
80.90	2857.0
81.90	676.0
86.90	2800.0
88.00	2657.0
90.90	339.0
92.00	2256.0
93.00	3322.0
94.00	8855.0
95.00	68304.0
96.00	4454.0
96.90	169.0
103.80	358.0
104.90	140.0
105.90	404.0
106.90	113.0
111.00	105.0
112.90	120.0
114.90	124.0
115.90	299.0
116.90	605.0
117.80	291.0
118.80	498.0
127.70	241.0
128.80	122.0
129.80	254.0
130.90	109.0
134.80	172.0
136.80	129.0
140.80	785.0
142.00	106.0
142.80	810.0
144.80	196.0
145.80	137.0
147.70	178.0
156.90	127.0
171.90	546.0
173.90	46344.0
174.90	3610.0
175.90	44648.0
176.90	2973.0
178.00	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

m/z	Abundance
36.00	574.0
37.00	3837.0
38.00	3491.0
39.00	1330.0
39.90	246.0
44.00	783.0
45.00	679.0
46.10	151.0
47.00	1018.0
47.90	345.0
49.00	3073.0
50.00	14274.0
51.00	4402.0
52.00	226.0
54.90	235.0
56.00	1153.0
57.00	2086.0
58.00	132.0
60.00	769.0
61.00	3651.0
62.00	3785.0
63.00	2877.0
64.00	336.0
65.00	322.0
65.90	109.0
67.00	149.0
68.00	7523.0
69.00	7658.0
70.00	639.0
71.90	522.0
73.00	3231.0
74.00	12729.0
75.00	35672.0
76.00	3258.0
76.90	412.0
77.90	257.0
78.90	2442.0
79.90	757.0
80.90	2574.0
81.80	610.0
86.90	2641.0
88.00	2744.0
90.80	354.0
91.90	2161.0
93.00	3337.0
94.00	8544.0
95.00	66440.0
96.00	4189.0
97.00	149.0
103.80	377.0
104.90	131.0
105.90	358.0
114.90	118.0
115.90	308.0
116.90	595.0
117.80	284.0
118.80	435.0
127.80	215.0
128.80	104.0
129.80	274.0
130.90	115.0
134.80	170.0
136.80	132.0
140.80	759.0
142.00	115.0
142.80	842.0
144.80	188.0
145.80	169.0
147.70	162.0
156.90	119.0
172.00	559.0
173.90	46368.0
174.90	3530.0
175.90	45256.0
176.90	3036.0
178.00	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

Scan 2788 (10.055 min): VV016215.D
BFB32

m/z	Abundance
39.80	197.0
44.00	228.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32