
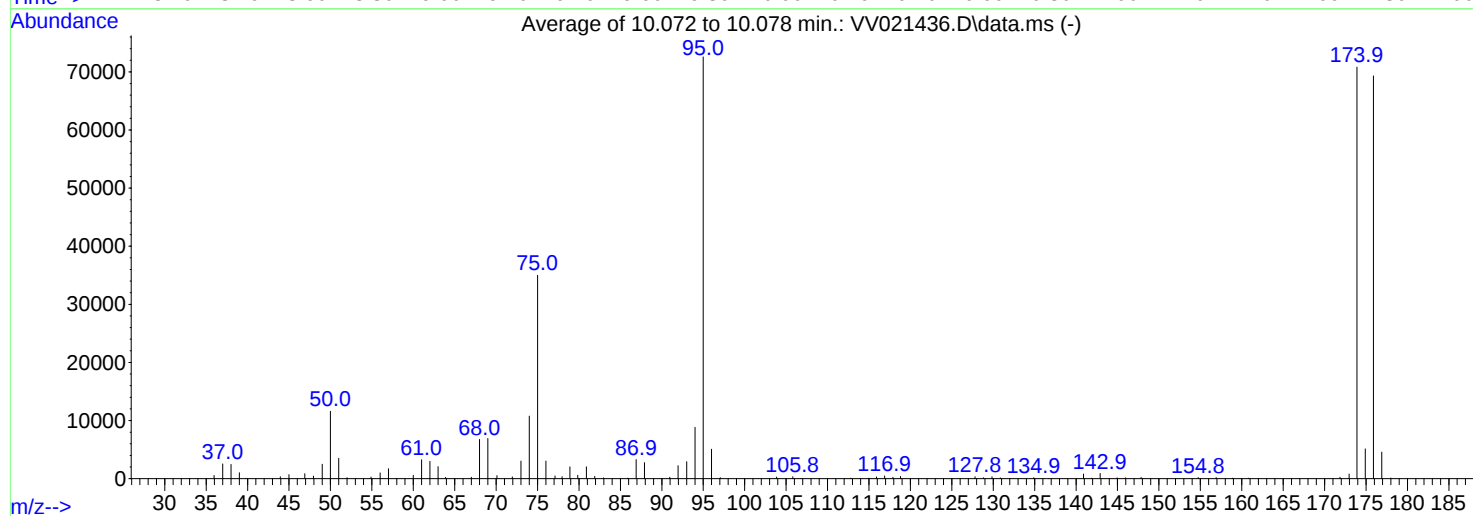


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052721\
 Data File : VV021436.D
 Acq On : 27 May 2021 09:44
 Operator : SY/MD
 Sample : BFB99
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB199

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis
 Last Update : Fri May 28 02:47:54 2021

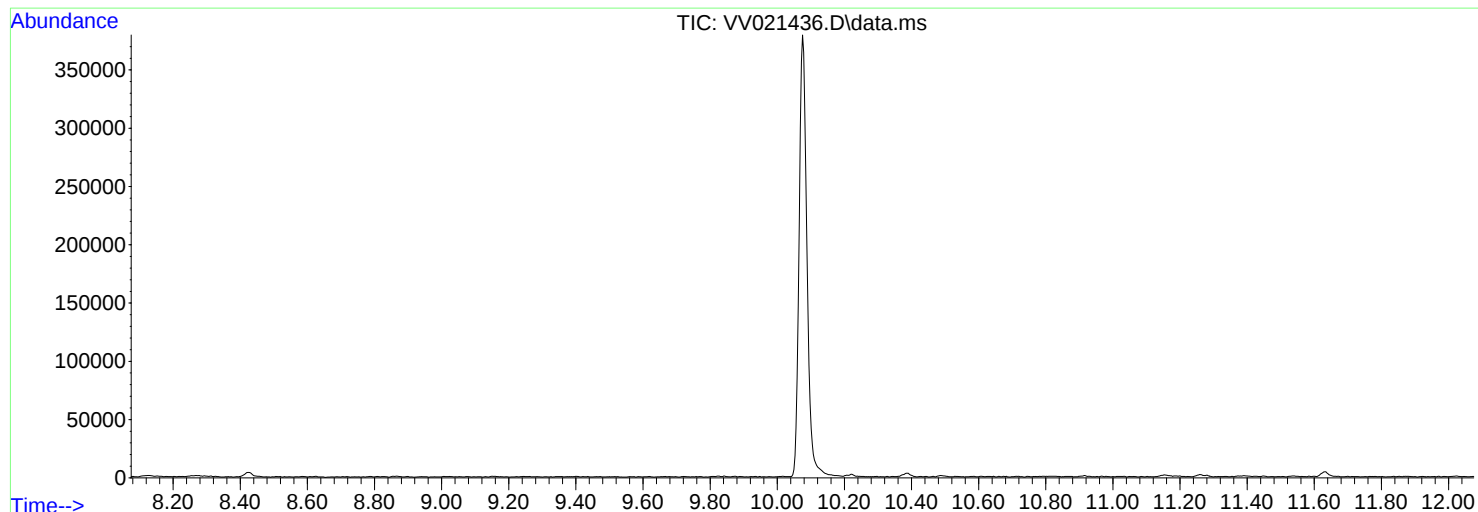

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	11590	PASS
75	95	30	80	48.2	35005	PASS
95	95	100	100	100.0	72592	PASS
96	95	5	9	7.0	5056	PASS
173	174	0.00	2	1.1	808	PASS
174	95	50	120	97.6	70835	PASS
175	174	5	9	7.2	5131	PASS
176	174	95	105	97.8	69304	PASS
177	176	5	10	6.6	4576	PASS

m/z	Abundance
36.00	497.0
37.00	2607.0
38.00	2284.0
39.00	1042.0
39.90	203.0
44.00	850.0
45.00	682.0
46.90	799.0
48.00	404.0
49.00	2419.0
50.00	11327.0
51.00	3403.0
52.00	190.0
54.90	226.0
56.00	980.0
57.00	1672.0
60.00	559.0
61.00	3231.0
62.00	2764.0
63.00	2156.0
63.90	206.0
67.00	218.0
68.00	6646.0
69.00	6800.0
70.10	454.0
72.00	320.0
73.00	3078.0
74.00	10473.0
75.00	34272.0
76.00	2861.0
77.10	445.0
78.00	351.0
78.90	1952.0
79.90	609.0
80.90	2100.0
81.90	376.0
82.90	118.0
86.90	3269.0
87.90	2747.0
91.00	214.0
91.90	2179.0
93.00	2857.0
94.00	8662.0
95.00	72224.0
96.00	4806.0
97.10	166.0
103.90	329.0
105.80	333.0
112.80	148.0
115.00	114.0
115.90	297.0
116.90	473.0
117.90	265.0
118.80	361.0
127.80	334.0
128.80	157.0
129.90	357.0
130.90	105.0
134.90	166.0
136.70	108.0
140.90	758.0
142.90	919.0
144.90	121.0
145.90	142.0
147.90	232.0
154.80	168.0
156.90	168.0
160.90	155.0
171.80	242.0
172.90	795.0
173.90	71104.0
174.90	5214.0
175.90	70208.0
176.90	4576.0
178.00	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB199

m/z	Abundance
36.00	563.0
37.00	2559.0
38.00	2531.0
39.00	1078.0
39.90	218.0
43.90	863.0
45.00	728.0
46.90	873.0
47.90	453.0
49.00	2605.0
50.00	11911.0
51.00	3558.0
52.00	163.0
54.90	268.0
56.00	1040.0
57.00	1802.0
60.00	602.0
61.00	3321.0
62.00	3082.0
63.00	2135.0
63.90	208.0
67.00	251.0
68.00	6956.0
69.00	7164.0
70.10	550.0
72.00	307.0
73.00	3130.0
74.00	11090.0
75.00	36232.0
76.00	3135.0
77.10	502.0
77.90	344.0
78.90	2127.0
79.90	602.0
80.90	2124.0
81.90	398.0
83.00	135.0
85.90	123.0
86.90	3457.0
87.90	2863.0
90.90	245.0
92.00	2291.0
93.00	2994.0
94.00	9151.0
95.00	75080.0
96.00	5191.0
97.00	159.0
103.80	278.0
105.80	332.0
112.80	105.0
115.00	107.0
115.90	318.0
116.90	491.0
117.90	267.0
118.80	406.0
127.80	350.0
128.80	175.0
129.90	349.0
130.90	140.0
134.90	167.0
140.90	842.0
141.80	107.0
142.90	922.0
144.90	155.0
146.00	133.0
147.90	231.0
154.70	183.0
156.90	199.0
158.90	125.0
160.80	103.0
171.90	269.0
173.00	838.0
173.90	73248.0
174.90	5258.0
175.90	71888.0
176.90	4718.0
178.00	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB199

m/z	Abundance
39.80	171.0
41.10	148.0
41.90	112.0
43.00	117.0
44.00	508.0

Instrument :
MSVOA_V
ClientSampleId :
BFB199

m/z	Abundance
35.00	565.0
37.00	2413.0
38.00	2566.0
39.00	967.0
39.80	239.0
43.10	108.0
43.90	842.0
45.00	621.0
46.90	878.0
47.90	455.0
49.00	2452.0
50.00	11532.0
51.00	3502.0
52.00	134.0
54.90	299.0
56.00	976.0
57.00	1667.0
58.00	102.0
60.00	569.0
61.00	3180.0
62.00	3100.0
63.00	1934.0
63.90	235.0
67.00	245.0
68.00	6616.0
69.00	6796.0
70.10	554.0
71.90	300.0
73.00	2854.0
74.00	10753.0
75.00	34512.0
76.00	3123.0
77.10	464.0
77.90	322.0
78.90	2048.0
79.80	571.0
80.90	1892.0
81.90	399.0
83.00	134.0
85.80	171.0
86.90	3126.0
87.90	2652.0
90.90	272.0
92.00	2215.0
93.00	2880.0
94.00	8718.0
95.00	70472.0
96.00	5171.0
97.00	143.0
103.80	244.0
105.80	294.0
106.80	123.0
115.90	297.0
116.90	447.0
117.90	256.0
118.80	438.0
127.80	324.0
128.80	176.0
129.80	301.0
130.80	143.0
134.90	157.0
140.90	818.0
141.90	129.0
142.90	858.0
145.00	158.0
146.00	143.0
147.80	198.0
154.70	193.0
156.90	177.0
158.90	128.0
171.90	221.0
173.00	791.0
173.90	68152.0
174.90	4920.0
175.90	65816.0
176.90	4433.0
178.00	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB199