


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052723\
 Data File : VV031249.D
 Acq On : 26 May 2023 13:19
 Operator : SY/MD
 Sample : BFB266
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB266

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052523WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat May 27 01:45:01 2023

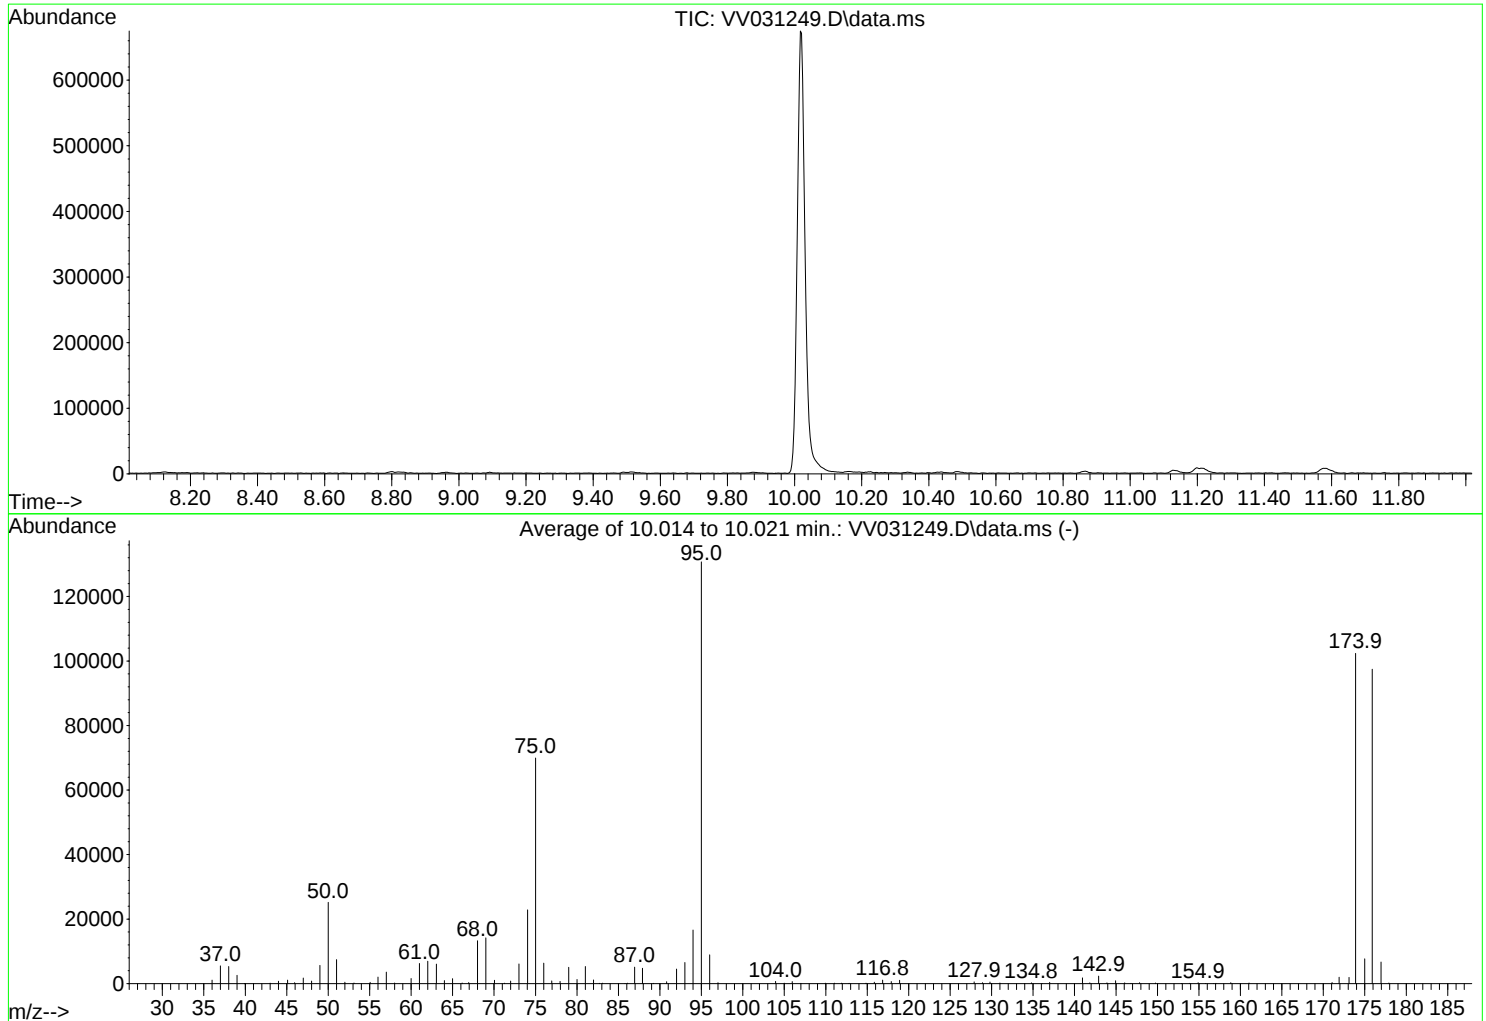

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	25179	PASS
75	95	30	80	53.5	69928	PASS
95	95	100	100	100.0	130739	PASS
96	95	5	9	6.8	8934	PASS
173	174	0.00	2	1.9	1961	PASS
174	95	50	120	78.3	102373	PASS
175	174	5	9	7.5	7668	PASS
176	174	95	105	95.2	97440	PASS
177	176	5	10	6.9	6687	PASS

m/z	Abundance
36.00	122.0
38.00	103.0
39.90	461.0
44.00	460.0
45.60	104.0
51.20	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB266

m/z	Abundance
36.00	1273.0
37.00	5034.0
38.00	4868.0
39.00	2355.0
40.00	539.0
41.00	108.0
43.00	129.0
44.00	1182.0
45.10	1114.0
46.00	356.0
47.00	1818.0
48.00	648.0
49.00	5418.0
50.00	24200.0
51.00	7275.0
52.00	474.0
53.10	191.0
55.00	431.0
56.00	1855.0
57.00	3557.0
58.00	164.0
60.00	1430.0
61.00	6038.0
62.00	6306.0
63.00	5932.0
64.00	932.0
65.00	1618.0
66.10	202.0
67.00	397.0
68.00	12654.0
69.00	13471.0
70.10	887.0
71.30	123.0
72.00	788.0
73.00	5868.0
74.10	21568.0
75.00	65168.0
76.00	5974.0
76.90	763.0
78.00	746.0
79.00	4753.0
80.00	1162.0
81.00	4845.0
82.00	1089.0
83.10	171.0
86.10	223.0
87.00	4798.0
87.90	4683.0
89.20	115.0
90.80	559.0
92.00	4000.0
93.00	6204.0
94.00	15449.0
95.00	122200.0
96.00	8685.0
97.00	332.0
103.90	650.0
104.90	221.0
105.90	623.0
110.00	129.0
111.00	172.0
111.90	141.0
114.90	175.0
115.90	444.0
116.80	1035.0
117.90	568.0
118.90	1003.0
127.90	456.0
128.90	256.0
129.80	428.0
131.10	146.0
134.80	196.0
137.00	369.0
141.00	1674.0
141.80	219.0
142.90	2297.0
143.90	167.0
144.90	804.0
146.10	318.0
147.90	242.0
149.80	145.0
154.90	307.0
157.10	181.0
158.90	269.0
161.10	157.0
171.00	356.0
171.90	1838.0
173.10	1708.0
173.90	94048.0
175.00	7283.0
175.90	89680.0
177.00	6285.0

Instrument :
MSVOA_V
ClientSampleId :
BFB266

177.90

223.0

Instrument :
MSVOA_V
ClientSampleId :
BFB266

m/z	Abundance
36.00	1239.0
37.00	5708.0
38.00	5558.0
39.00	2717.0
40.00	504.0
43.00	152.0
44.00	1250.0
45.10	1121.0
45.90	303.0
47.00	1818.0
48.00	837.0
49.00	5857.0
50.00	26216.0
51.00	7765.0
52.00	512.0
53.10	188.0
55.00	415.0
56.00	2103.0
57.00	3741.0
58.00	180.0
60.00	1649.0
61.00	6528.0
62.00	7245.0
63.10	6295.0
64.00	1011.0
65.00	1557.0
66.10	184.0
67.00	359.0
68.00	13747.0
69.00	14784.0
70.00	1086.0
71.20	188.0
72.00	795.0
73.00	6328.0
74.00	23704.0
75.00	72184.0
76.00	6647.0
76.90	880.0
78.00	699.0
79.00	5290.0
80.00	1331.0
81.00	5464.0
82.00	1233.0
82.70	136.0
83.10	177.0
86.10	236.0
87.00	5273.0
87.90	4955.0
89.20	131.0
90.80	618.0
92.00	4702.0
93.00	6881.0
94.00	17280.0
95.00	135168.0
96.00	9275.0
97.00	317.0
104.00	679.0
105.00	177.0
105.90	684.0
107.00	137.0
110.00	135.0
111.00	159.0
111.90	151.0
112.80	119.0
114.80	176.0
115.90	475.0
116.80	1125.0
117.90	690.0
118.90	1096.0
127.90	581.0
128.90	301.0
129.80	552.0
131.00	183.0
134.80	241.0
137.00	428.0
140.90	1891.0
141.90	258.0
142.90	2406.0
143.90	278.0
144.90	977.0
146.00	294.0
146.80	142.0
147.90	314.0
149.70	187.0
153.90	159.0
154.90	295.0
157.00	183.0
158.80	303.0
161.10	199.0
171.10	352.0
171.90	2060.0
173.10	2067.0

Instrument :
MSVOA_V
ClientSampleId :
BFB266

173.90	105824.0
175.00	7813.0
175.90	101112.0
176.90	6935.0
177.90	232.0

Instrument :
MSVOA_V
ClientSampleId :
BFB266

m/z	Abundance
36.00	1178.0
37.00	5792.0
38.00	5828.0
39.00	2748.0
39.90	372.0
43.00	148.0
44.00	1199.0
45.10	1020.0
45.90	215.0
47.00	1530.0
48.00	852.0
49.00	5694.0
50.00	25120.0
51.00	7659.0
52.00	438.0
53.10	200.0
55.10	379.0
56.00	2120.0
57.00	3464.0
58.00	198.0
60.00	1655.0
61.00	6201.0
62.00	7294.0
63.10	6003.0
64.00	979.0
65.00	1416.0
66.20	174.0
66.90	306.0
68.00	13481.0
69.00	14290.0
70.00	1190.0
71.20	181.0
72.00	782.0
73.00	6128.0
74.00	23384.0
75.00	72432.0
76.00	6434.0
77.00	870.0
77.90	613.0
79.00	5148.0
80.00	1389.0
81.00	5647.0
82.00	1171.0
82.70	137.0
83.10	156.0
85.80	212.0
86.90	5228.0
87.90	4617.0
90.80	604.0
92.00	4837.0
93.00	6630.0
94.00	17160.0
95.00	134848.0
96.00	8843.0
97.00	260.0
104.00	692.0
105.10	128.0
106.00	694.0
107.00	165.0
109.90	137.0
111.10	122.0
111.90	138.0
112.80	137.0
114.80	158.0
115.80	504.0
116.90	1096.0
117.90	739.0
118.90	1044.0
127.90	576.0
128.90	282.0
129.80	574.0
130.90	217.0
134.00	113.0
134.80	260.0
136.10	141.0
137.00	331.0
140.90	1831.0
141.80	250.0
142.90	2362.0
143.90	334.0
145.00	942.0
146.00	202.0
146.80	166.0
147.80	343.0
149.70	195.0
152.90	101.0
153.90	189.0
154.90	276.0
155.80	115.0
156.80	171.0
158.80	287.0
161.00	210.0

Instrument :
MSVOA_V
ClientSampleId :
BFB266

171.10	354.0
171.90	2086.0
173.10	2108.0
173.90	107248.0
175.00	7909.0
175.90	101528.0
176.90	6840.0
177.90	228.0

Instrument :
MSVOA_V
ClientSampleId :
BFB266