

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052819\
 Data File : VV011066.D
 Acq On : 28 May 2019 16:34
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK

Quant Time: May 29 02:44:59 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM052819S.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 29 02:15:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	466813	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	443405	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	201265	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	157907	24.67	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.68%
7) Chloroethane-d5	1.57	69	112247	24.57	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.28%
10) 1,1-Dichloroethene-d2	2.12	63	234878	19.73	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	78.92%
20) 2-Butanone-d5	3.93	46	122526	55.54	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.08%
24) Chloroform-d	4.40	84	208939	18.46	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	73.84%
26) 1,2-Dichloroethane-d4	5.08	65	176331	24.36	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.44%
29) Benzene-d6	5.09	84	627566	24.17	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.68%
33) 1,2-Dichloropropane-d6	6.11	67	199585	24.16	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.64%
37) Toluene-d8	7.36	98	595336	24.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.52%
38) trans-1,3-Dichloropropene-	7.66	79	90433	23.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.00%
39) 2-Hexanone-d5	8.13	63	95118	52.86	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.72%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	170539	24.01	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.04%
61) 1,2-Dichlorobenzene-d4	11.67	152	189461	23.81	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.24%


Target Compounds					Ovalue
13) Acetone	2.19	43	10083	4.035 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052819\
Data File : VV011066.D
Acq On : 28 May 2019 16:34
Operator : SY/MD
Sample : VIBLK
Misc : 5.00G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Quant Time: May 29 02:44:59 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM052819S.M
Quant Title : VOC Analysis
QLast Update : Wed May 29 02:15:20 2019
Response via : Initial Calibration

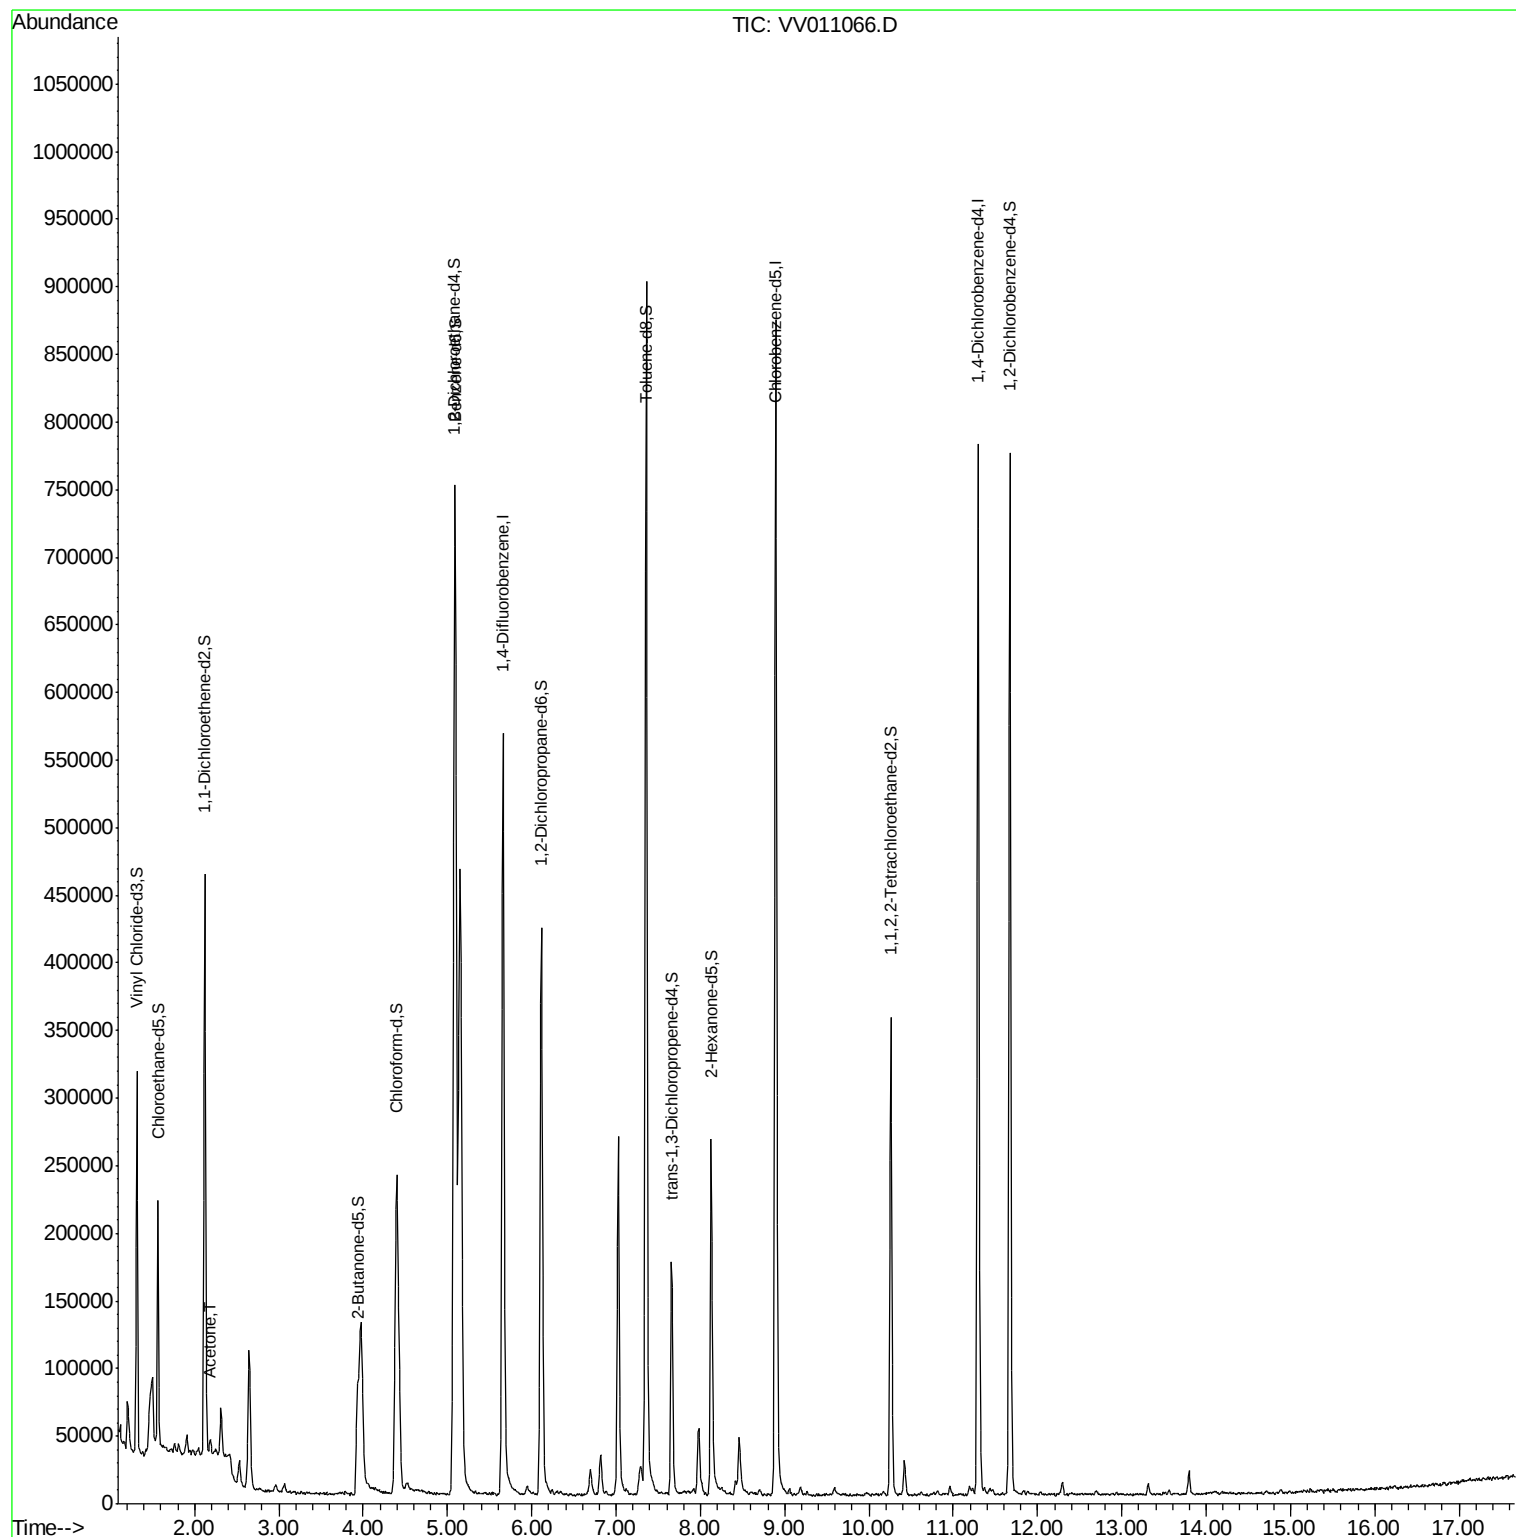

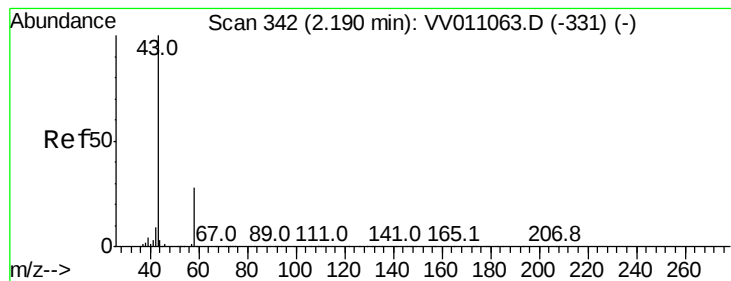

#13

Acetone

Concen: 4.035 ug/L

RT: 2.19 min Scan# 342

Delta R.T. -0.00 min

Lab File: VV011066.D

Acq: 28 May 2019 16:34

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Tot Ion: 43 Resp: 10083

Ion Ratio Lower Upper

43 100

58 26.6 0.0 54.8

