


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052819\
Data File : VV011056.D
Acq On : 28 May 2019 09:15
Operator : SY/MD
Sample : BFB64
Misc : 5.00G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB64

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM052819S.M
Title : VOC Analysis
Last Update : Thu May 30 04:49:33 2019

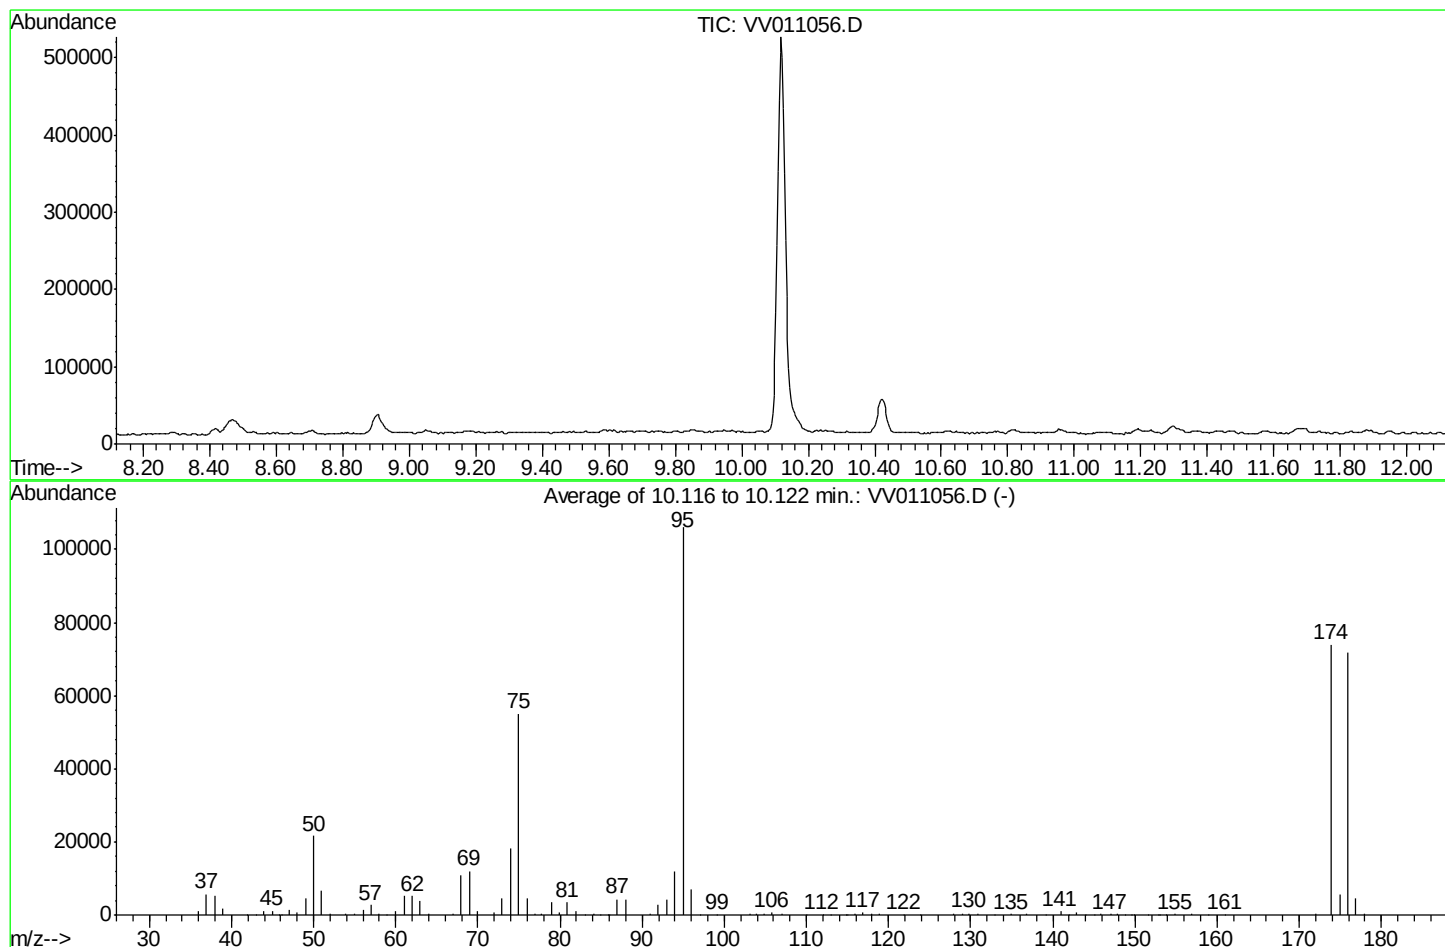

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	21696	PASS
75	95	30	80	51.8	54977	PASS
95	95	100	100	100.0	106052	PASS
96	95	5	9	6.6	7010	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.7	73898	PASS
175	174	5	9	7.6	5633	PASS
176	174	95	101	97.3	71896	PASS
177	176	5	9	6.3	4499	PASS

m/z	Abundance
36.00	1950.0
36.90	251.0
37.90	962.0
39.00	543.0
39.90	634.0
41.10	803.0
42.00	329.0
43.10	781.0
43.90	1054.0
45.00	195.0
48.70	119.0
50.00	154.0
51.00	157.0
52.00	110.0
53.00	218.0
54.20	157.0
55.00	577.0
56.10	305.0
57.00	620.0
59.90	131.0
62.90	112.0
65.00	110.0
66.00	119.0
66.90	252.0
67.90	177.0
69.00	385.0
70.00	170.0
71.00	292.0
72.90	170.0
74.80	116.0
77.00	220.0
77.50	124.0
78.00	112.0
78.90	152.0
80.10	125.0
81.00	170.0
82.20	122.0
82.90	271.0
85.00	132.0
90.90	151.0
92.00	126.0
94.00	113.0
95.00	174.0
95.90	217.0
97.10	234.0
97.90	256.0
105.00	102.0
109.20	103.0
110.30	111.0
111.10	193.0
119.00	288.0
168.90	468.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
36.00	3075.0
37.00	6084.0
38.00	6092.0
39.00	2496.0
40.00	530.0
41.00	617.0
41.90	412.0
42.90	882.0
43.90	2138.0
44.90	1263.0
45.80	143.0
46.20	156.0
47.00	1469.0
48.00	866.0
49.00	4885.0
50.00	21664.0
51.00	6767.0
52.00	417.0
52.80	168.0
53.90	220.0
55.00	1080.0
56.00	1951.0
57.00	3529.0
58.00	272.0
58.90	140.0
59.90	1067.0
61.00	5208.0
62.00	5097.0
63.00	3982.0
64.00	439.0
65.00	132.0
67.00	493.0
68.00	11055.0
69.00	12142.0
69.90	996.0
71.10	270.0
72.00	666.0
73.00	4586.0
74.00	18024.0
75.00	55168.0
76.00	4605.0
77.00	802.0
77.80	467.0
78.90	3622.0
79.90	889.0
80.90	3528.0
81.90	974.0
83.00	379.0
84.10	282.0
85.00	216.0
85.80	207.0
87.00	4288.0
88.00	4092.0
91.00	494.0
91.90	2941.0
93.00	4270.0
94.00	11857.0
95.00	105664.0
96.00	7206.0
96.90	390.0
98.00	221.0
103.10	184.0
103.90	515.0
104.90	276.0
105.80	515.0
107.00	230.0
110.00	156.0
111.00	174.0
113.00	201.0
114.70	160.0
115.00	126.0
115.90	538.0
116.90	585.0
117.90	379.0
118.90	785.0
121.90	126.0
123.90	106.0
127.90	362.0
129.00	302.0
129.80	466.0
130.80	255.0
132.90	111.0
135.00	190.0
136.80	193.0
139.20	104.0
141.00	1050.0
141.80	123.0
142.90	876.0
143.90	106.0
145.00	100.0
145.90	187.0
147.00	160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

147.90	218.0
149.60	114.0
151.70	142.0
152.80	128.0
153.80	105.0
154.90	343.0
156.90	252.0
158.90	167.0
160.90	120.0
169.00	224.0
172.10	216.0
173.90	71552.0
174.90	5404.0
175.90	69904.0
176.90	4577.0
177.90	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
36.00	3175.0
37.00	6153.0
38.00	6350.0
39.00	2487.0
40.00	535.0
41.00	601.0
41.90	379.0
42.90	913.0
44.00	2011.0
45.00	1280.0
46.00	142.0
47.00	1447.0
48.00	701.0
49.00	4827.0
50.00	22632.0
51.00	6899.0
52.00	412.0
52.80	171.0
53.90	219.0
55.00	1076.0
56.00	1948.0
57.00	3458.0
58.00	243.0
58.80	129.0
59.90	1087.0
61.00	5345.0
62.00	5377.0
63.00	4075.0
64.00	485.0
65.00	112.0
67.00	519.0
68.00	11248.0
69.00	12751.0
70.00	1121.0
71.00	275.0
72.00	634.0
73.00	4819.0
74.00	18760.0
75.00	56712.0
76.00	4575.0
77.00	709.0
77.80	469.0
78.90	3679.0
79.90	911.0
80.90	3681.0
81.90	970.0
83.00	367.0
84.10	217.0
84.90	236.0
86.00	196.0
86.90	4507.0
88.00	4202.0
90.90	524.0
91.90	3028.0
93.00	4402.0
94.00	12278.0
95.00	109248.0
96.00	7482.0
97.00	382.0
98.00	266.0
99.10	125.0
103.00	202.0
103.90	539.0
104.90	328.0
105.80	576.0
107.00	218.0
110.00	165.0
111.00	182.0
113.00	187.0
114.80	180.0
115.90	576.0
116.90	646.0
117.90	456.0
118.90	834.0
121.90	109.0
127.80	415.0
129.00	300.0
129.80	499.0
130.80	223.0
132.90	126.0
135.00	222.0
136.80	215.0
139.00	103.0
141.00	1093.0
141.90	158.0
142.90	904.0
145.00	135.0
145.90	203.0
147.00	233.0
147.90	227.0
149.80	107.0
151.60	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

153.00	130.0
154.90	334.0
156.90	243.0
158.90	178.0
160.90	119.0
169.00	234.0
172.00	248.0
173.90	76112.0
174.90	5870.0
175.90	74400.0
176.90	4621.0
177.90	207.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

m/z	Abundance
36.00	3033.0
37.00	5591.0
38.00	5898.0
39.00	2288.0
40.00	548.0
40.90	642.0
41.90	366.0
42.90	905.0
44.00	1899.0
45.00	1243.0
45.90	117.0
47.00	1278.0
47.90	639.0
49.00	4238.0
50.00	21256.0
51.00	6356.0
52.00	343.0
52.80	187.0
53.90	216.0
55.00	956.0
56.00	1769.0
57.00	3170.0
58.00	202.0
58.80	118.0
59.90	955.0
61.00	4966.0
62.00	5051.0
63.00	3717.0
64.00	451.0
66.90	512.0
68.00	10388.0
69.00	12027.0
70.00	1109.0
71.00	297.0
71.90	535.0
73.00	4798.0
74.00	17528.0
75.00	53400.0
76.00	4254.0
76.90	630.0
77.80	410.0
78.90	3335.0
80.00	879.0
80.90	3419.0
81.90	852.0
83.00	330.0
84.10	181.0
85.00	230.0
86.00	184.0
86.90	4242.0
88.00	4022.0
91.00	507.0
91.90	2844.0
93.00	4172.0
94.00	11805.0
95.00	103768.0
96.00	6993.0
97.00	391.0
98.00	254.0
99.10	148.0
103.00	184.0
103.80	450.0
104.90	375.0
105.90	558.0
107.00	150.0
109.10	126.0
109.90	141.0
111.10	145.0
112.00	135.0
112.80	138.0
114.90	206.0
115.80	493.0
116.80	645.0
117.90	517.0
118.80	800.0
127.80	392.0
129.00	280.0
129.90	480.0
130.80	212.0
132.90	117.0
134.90	241.0
136.80	198.0
140.90	1011.0
141.90	175.0
142.80	869.0
145.00	141.0
145.90	186.0
147.00	265.0
147.80	208.0
148.80	110.0
149.90	165.0
153.00	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64

154.90	329.0
156.90	207.0
158.80	148.0
161.00	110.0
169.00	227.0
172.00	230.0
173.90	74032.0
175.00	5625.0
175.90	71384.0
176.90	4301.0
177.90	213.0

Instrument :
MSVOA_V
ClientSampleId :
BFB64