

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052820\
 Data File : VV016277.D
 Acq On : 28 May 2020 15:21
 Operator : SY/MD
 Sample : L2756-02
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKW6

Quant Time: May 29 02:28:07 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR052620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 29 01:10:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	91915	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	90268	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	40268	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	21848	3.70	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.00%
7) Chloroethane-d5	1.58	69	21296	4.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.20%
11) 1,1-Dichloroethene-d2	2.13	63	33073	2.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.60%#
20) 2-Butanone-d5	3.94	46	71474	48.81	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.62%
24) Chloroform-d	4.38	84	50292	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.60%
26) 1,2-Dichloroethane-d4	5.06	65	28047	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.20%
32) Benzene-d6	5.08	84	95770	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.60%
36) 1,2-Dichloropropane-d6	6.10	67	31020	4.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.60%
41) Toluene-d8	7.34	98	86987	4.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.60%
45) trans-1,3-Dichloropropene-	7.65	79	9833	3.81	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.20%
48) 2-Hexanone-d5	8.12	63	51449	43.50	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.00%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	22173	4.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.80%
65) 1,2-Dichlorobenzene-d4	11.65	152	31479	4.68	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.60%


Target Compounds					Ovalue
13) Acetone	2.21	43	4336	4.784 ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052820\
Data File : VV016277.D
Acq On : 28 May 2020 15:21
Operator : SY/MD
Sample : L2756-02
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETKW6

Quant Time: May 29 02:28:07 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR052620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 29 01:10:53 2020
Response via : Initial Calibration

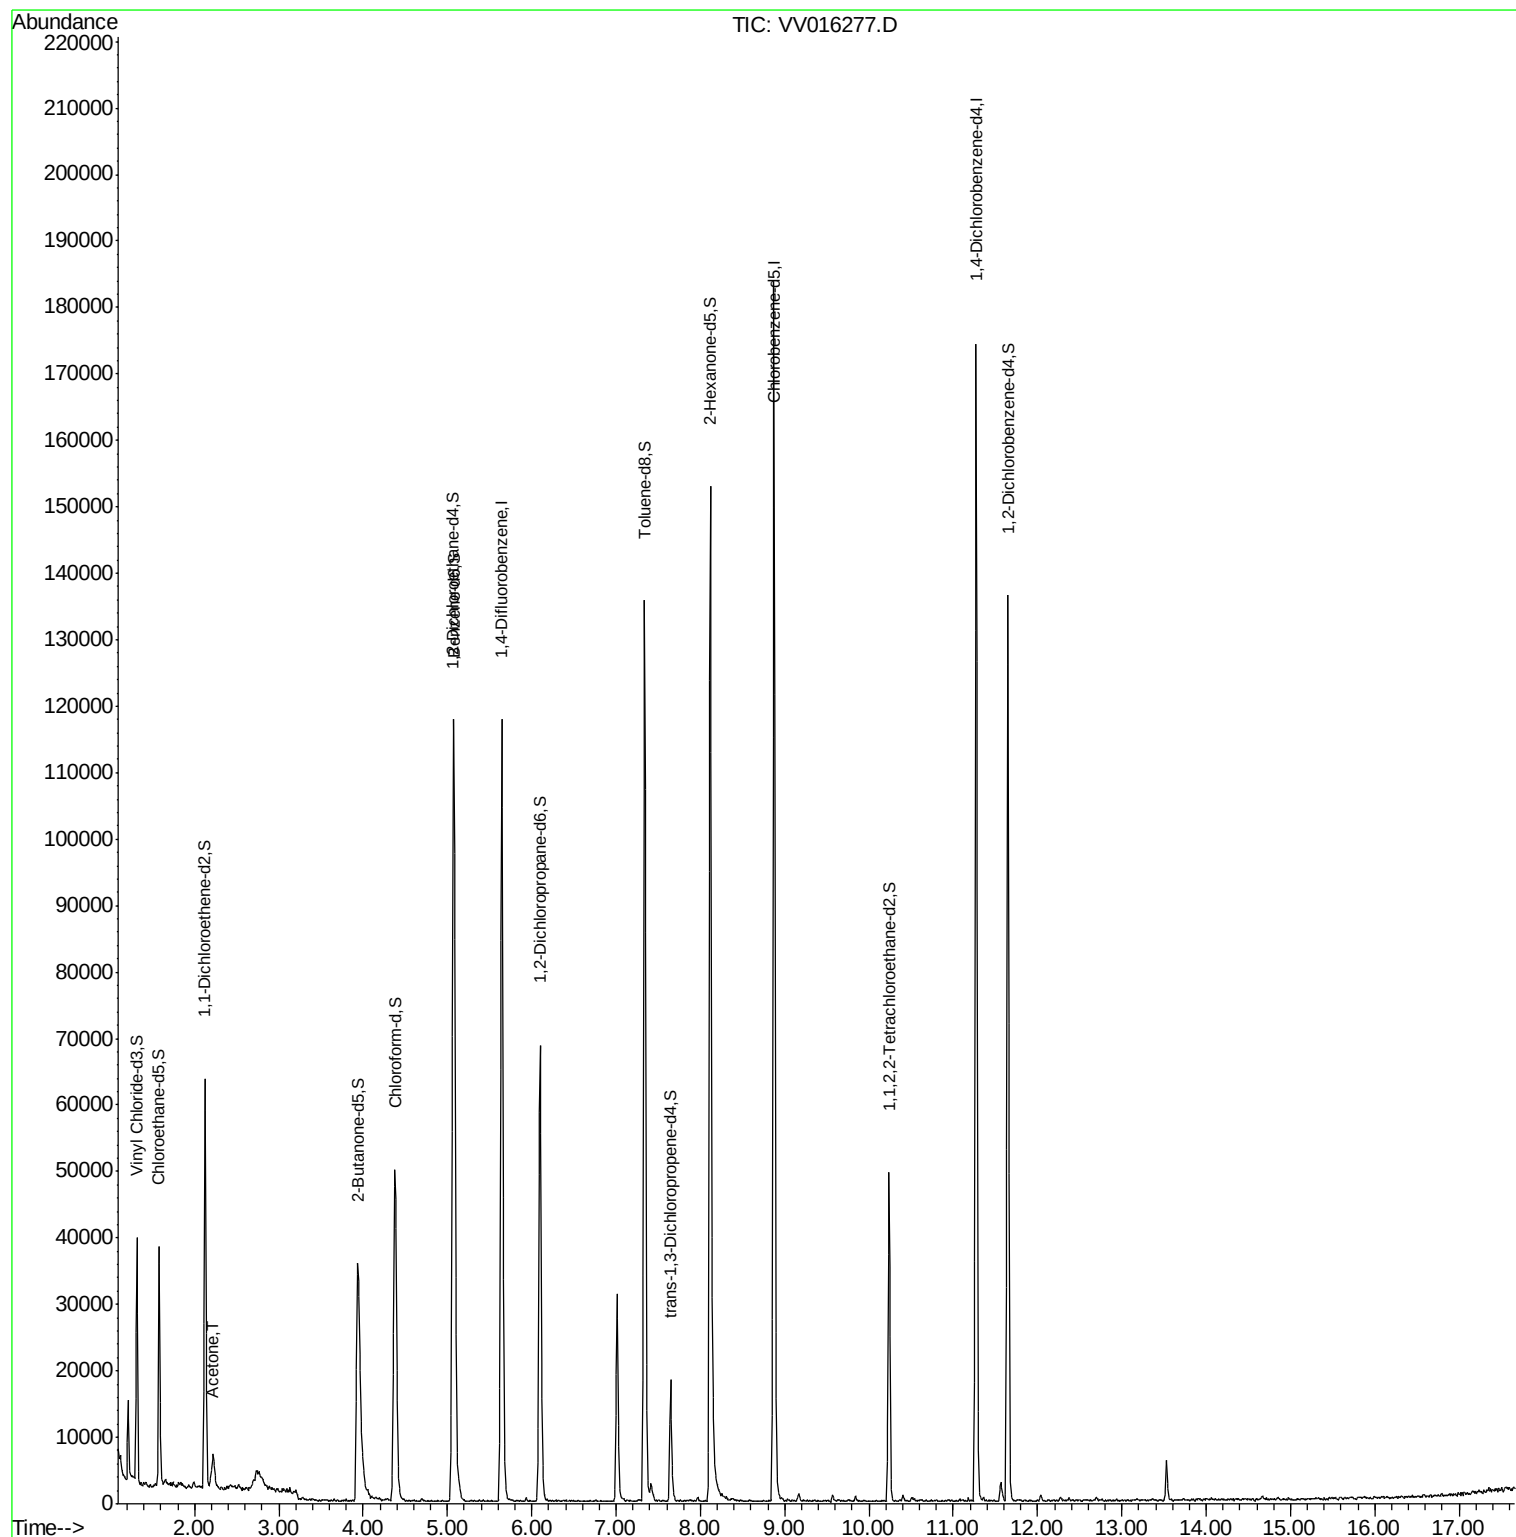

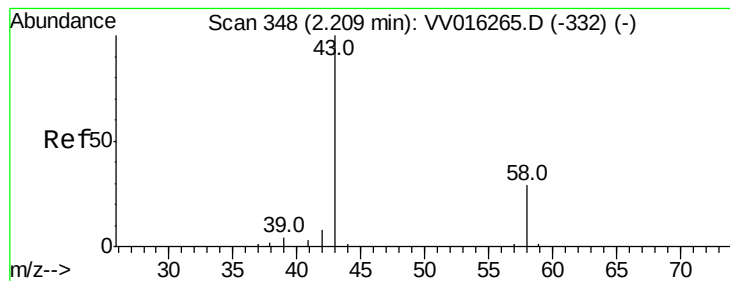

#13
 Acetone
 Concen: 4.784 ug/L
 RT: 2.21 min Scan# 347
 Delta R.T. -0.00 min
 Lab File: VV016277.D
 Acq: 28 May 2020 15:21

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKW6

Tot Ion: 43 Resp: 4336
 Ion Ratio Lower Upper
 43 100
 58 16.1 0.0 48.8

