

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052821\
 Data File : VV021449.D
 Acq On : 28 May 2021 10:45
 Operator : SY/MD
 Sample : VV0528WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK182

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	222541	222416	12.99%	1.609%
2	1.568	157	164	177	rVB	176815	202207	11.81%	1.463%
3	2.108	322	332	359	rVB	364712	550522	32.15%	3.983%
4	2.667	503	506	508	rBV3	428	259	0.02%	0.002%
5	2.761	532	535	537	rBV3	1741	1373	0.08%	0.010%
6	2.844	556	561	562	rBV2	523	417	0.02%	0.003%
7	2.883	569	573	576	rVB2	378	289	0.02%	0.002%
8	2.915	580	583	585	rBV3	415	290	0.02%	0.002%
9	3.169	659	662	663	rBV3	423	222	0.01%	0.002%
10	3.233	679	682	686	rBV4	312	215	0.01%	0.002%
11	3.288	696	699	707	rVB3	456	424	0.02%	0.003%
12	3.323	707	710	712	rBV	403	222	0.01%	0.002%
13	3.378	722	727	730	rBV3	317	320	0.02%	0.002%
14	3.423	739	741	743	rVB	356	178	0.01%	0.001%
15	3.436	743	745	749	rBV2	567	360	0.02%	0.003%
16	3.494	758	763	767	rBV2	594	650	0.04%	0.005%
17	3.513	767	769	772	rVB2	395	207	0.01%	0.001%
18	3.532	772	775	779	rBV2	296	268	0.02%	0.002%
19	3.658	809	814	815	rBV	299	256	0.01%	0.002%
20	3.693	822	825	828	rBV	285	197	0.01%	0.001%
21	3.709	828	830	833	rVB3	409	224	0.01%	0.002%
22	3.728	833	836	839	rBV2	283	168	0.01%	0.001%
23	3.783	852	853	855	rBV2	396	165	0.01%	0.001%
24	3.812	860	862	866	rVV2	404	228	0.01%	0.002%
25	3.892	875	887	925	rBV2	120858	411132	24.01%	2.974%
26	4.349	1013	1029	1062	rVB2	270979	669887	39.13%	4.846%
27	4.815	1172	1174	1175	rBV	607	237	0.01%	0.002%
28	4.937	1208	1212	1218	rVB3	448	404	0.02%	0.003%
29	5.047	1228	1246	1281	rBV2	669869	1712160	100.00%	12.386%
30	5.484	1378	1382	1385	rBV3	987	809	0.05%	0.006%
31	5.529	1393	1396	1402	rVB3	661	576	0.03%	0.004%
32	5.616	1410	1423	1455	rBV	532614	1080188	63.09%	7.814%
33	5.822	1486	1487	1489	rBV2	412	182	0.01%	0.001%
34	5.908	1504	1514	1532	rVB7	8512	18201	1.06%	0.132%
35	5.995	1537	1541	1542	rBV2	466	226	0.01%	0.002%
36	6.069	1550	1564	1594	rBV	370790	763462	44.59%	5.523%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052821\
 Data File : VV021449.D
 Acq On : 28 May 2021 10:45
 Operator : SY/MD
 Sample : VV0528WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK182

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.461	1683	1686	1690	rVB4	316	269	0.02%	0.002%
38	6.494	1693	1696	1697	rBV3	411	235	0.01%	0.002%
39	6.587	1722	1725	1728	rVB	317	157	0.01%	0.001%
40	6.648	1734	1744	1747	rBV8	1616	2678	0.16%	0.019%
41	6.793	1786	1789	1791	rBV2	364	240	0.01%	0.002%
42	6.841	1800	1804	1808	rBV3	383	413	0.02%	0.003%
43	6.876	1811	1815	1821	rVB4	418	408	0.02%	0.003%
44	6.915	1821	1827	1830	rVB2	438	464	0.03%	0.003%
45	6.934	1830	1833	1835	rBV3	455	275	0.02%	0.002%
46	6.985	1838	1849	1875	rBV	241090	437770	25.57%	3.167%
47	7.159	1901	1903	1907	rVB3	586	247	0.01%	0.002%
48	7.317	1940	1952	1967	rBV	833183	1449524	84.66%	10.486%
49	7.622	2036	2047	2076	rBV	165459	292308	17.07%	2.115%
50	7.979	2152	2158	2166	rVB7	2025	2906	0.17%	0.021%
51	8.021	2167	2171	2176	rVB3	704	705	0.04%	0.005%
52	8.088	2182	2192	2222	rBV	487657	860716	50.27%	6.227%
53	8.465	2307	2309	2313	rBV3	582	386	0.02%	0.003%
54	8.616	2354	2356	2358	rBV2	306	172	0.01%	0.001%
55	8.780	2404	2407	2409	rBV	233	168	0.01%	0.001%
56	8.799	2411	2413	2416	rVB2	341	164	0.01%	0.001%
57	8.854	2416	2430	2458	rBV	778066	1287143	75.18%	9.312%
58	9.018	2477	2481	2483	rBV2	2158	1929	0.11%	0.014%
59	9.072	2496	2498	2500	rBV2	444	183	0.01%	0.001%
60	9.149	2513	2522	2531	rBV5	3218	6289	0.37%	0.045%
61	9.194	2534	2536	2540	rVB2	603	229	0.01%	0.002%
62	9.252	2553	2554	2560	rVB3	423	200	0.01%	0.001%
63	9.326	2573	2577	2580	rBV3	273	253	0.01%	0.002%
64	9.387	2593	2596	2600	rBV2	335	241	0.01%	0.002%
65	9.493	2627	2629	2632	rVB	273	165	0.01%	0.001%
66	9.522	2632	2638	2639	rBV3	566	443	0.03%	0.003%
67	9.548	2641	2646	2651	rBV5	2850	3634	0.21%	0.026%
68	9.673	2682	2685	2687	rBV3	585	457	0.03%	0.003%
69	9.738	2700	2705	2714	rVB3	755	986	0.06%	0.007%
70	9.847	2734	2739	2743	rBV2	401	504	0.03%	0.004%
71	9.937	2759	2767	2776	rBV3	2708	4451	0.26%	0.032%
72	10.021	2788	2793	2799	rBV3	438	456	0.03%	0.003%
73	10.059	2802	2805	2806	rBV	289	163	0.01%	0.001%
74	10.127	2814	2826	2835	rVB3	4559	7365	0.43%	0.053%
75	10.217	2841	2854	2880	rBV	573355	897397	52.41%	6.492%
76	10.413	2912	2915	2921	rBV4	385	372	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052821\
 Data File : VV021449.D
 Acq On : 28 May 2021 10:45
 Operator : SY/MD
 Sample : VV0528WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK182

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	10.439	2921	2923	2925	rBV3	272	168	0.01%	0.001%
78	10.481	2935	2936	2940	rVB3	609	263	0.02%	0.002%
79	10.545	2945	2956	2960	rBV6	3098	4986	0.29%	0.036%
80	10.886	3056	3062	3063	rBV3	734	662	0.04%	0.005%
81	10.918	3067	3072	3084	rVB5	7631	11543	0.67%	0.084%
82	11.146	3133	3143	3149	rBV5	2492	3949	0.23%	0.029%
83	11.188	3149	3156	3164	rBV5	2936	4689	0.27%	0.034%
84	11.249	3164	3175	3195	rBV	905742	1416541	82.73%	10.248%
85	11.625	3280	3292	3318	rBV	912275	1436448	83.90%	10.392%
86	11.892	3372	3375	3382	rBV3	449	518	0.03%	0.004%
87	11.943	3386	3391	3394	rBV3	625	426	0.02%	0.003%
88	11.982	3400	3403	3406	rBV3	845	616	0.04%	0.004%
89	12.095	3436	3438	3441	rBV3	496	383	0.02%	0.003%
90	12.130	3446	3449	3454	rBV5	504	430	0.03%	0.003%
91	12.313	3504	3506	3509	rBV2	658	350	0.02%	0.003%
92	12.378	3521	3526	3530	rBV5	610	679	0.04%	0.005%
93	12.435	3538	3544	3551	rVB6	1193	1670	0.10%	0.012%
94	12.464	3551	3553	3555	rBV6	291	171	0.01%	0.001%
95	13.220	3786	3788	3795	rVB3	499	441	0.03%	0.003%
96	13.268	3795	3803	3811	rBV5	6427	9623	0.56%	0.070%
97	13.400	3842	3844	3846	rBV2	505	305	0.02%	0.002%
98	13.513	3872	3879	3894	rVB3	7345	12980	0.76%	0.094%
99	13.750	3945	3953	3967	rVB3	7389	12070	0.70%	0.087%
100	13.863	3986	3988	3993	rBV	702	430	0.03%	0.003%




Sum of corrected areas: 13822947

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052821\
Data File : VV021449.D
Acq On : 28 May 2021 10:45
Operator : SY/MD
Sample : VV0528WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK182

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

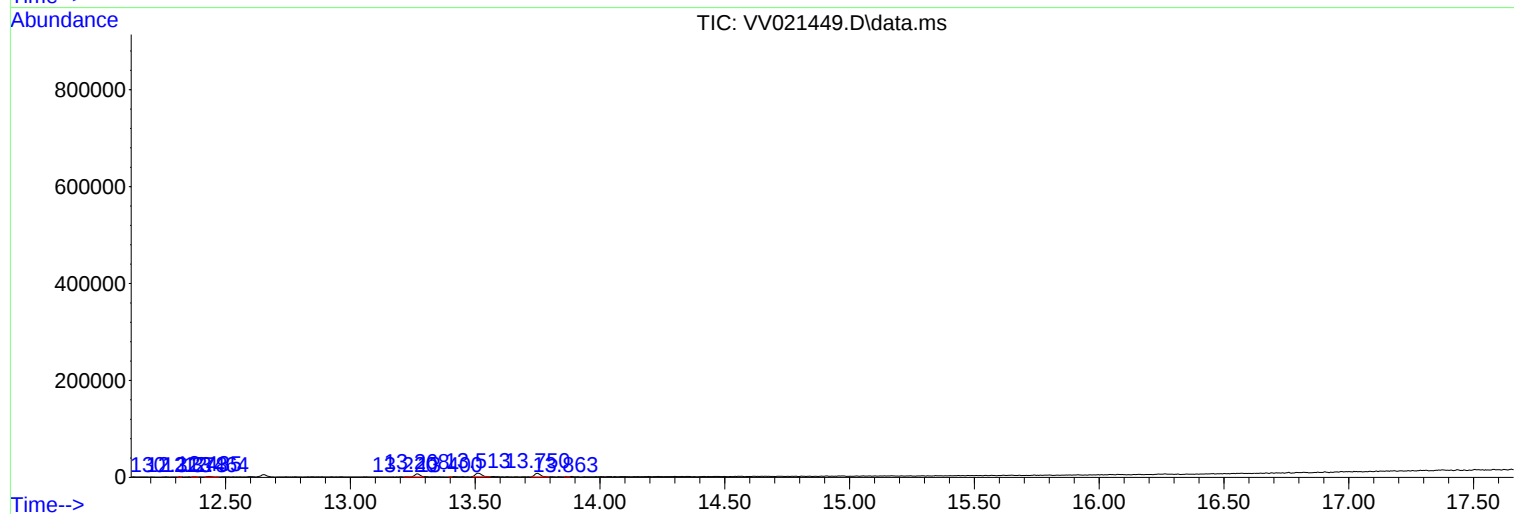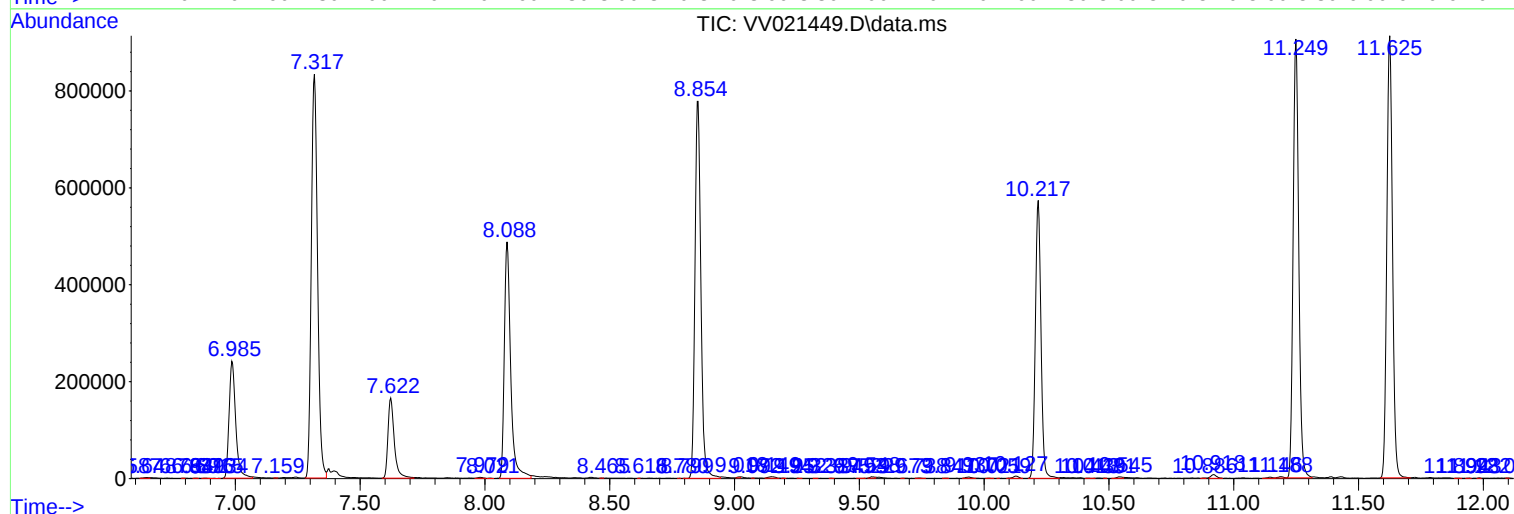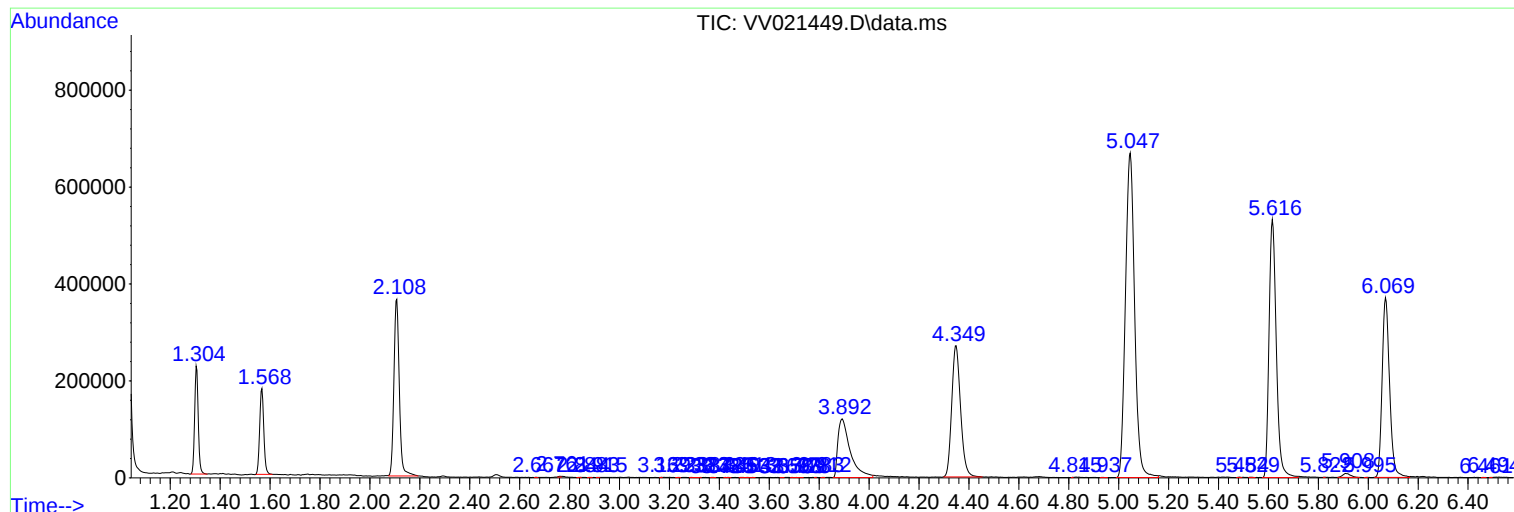

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052821\
Data File : VV021449.D
Acq On : 28 May 2021 10:45
Operator : SY/MD
Sample : VV0528WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK182

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052821\
Data File : VV021449.D
Acq On : 28 May 2021 10:45
Operator : SY/MD
Sample : VV0528WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK182

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
