


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052821\
Data File : VV021447.D
Acq On : 28 May 2021 09:18
Operator : SY/MD
Sample : BFB61
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB161

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Title : VOC Analysis
Last Update : Sat May 29 00:49:04 2021

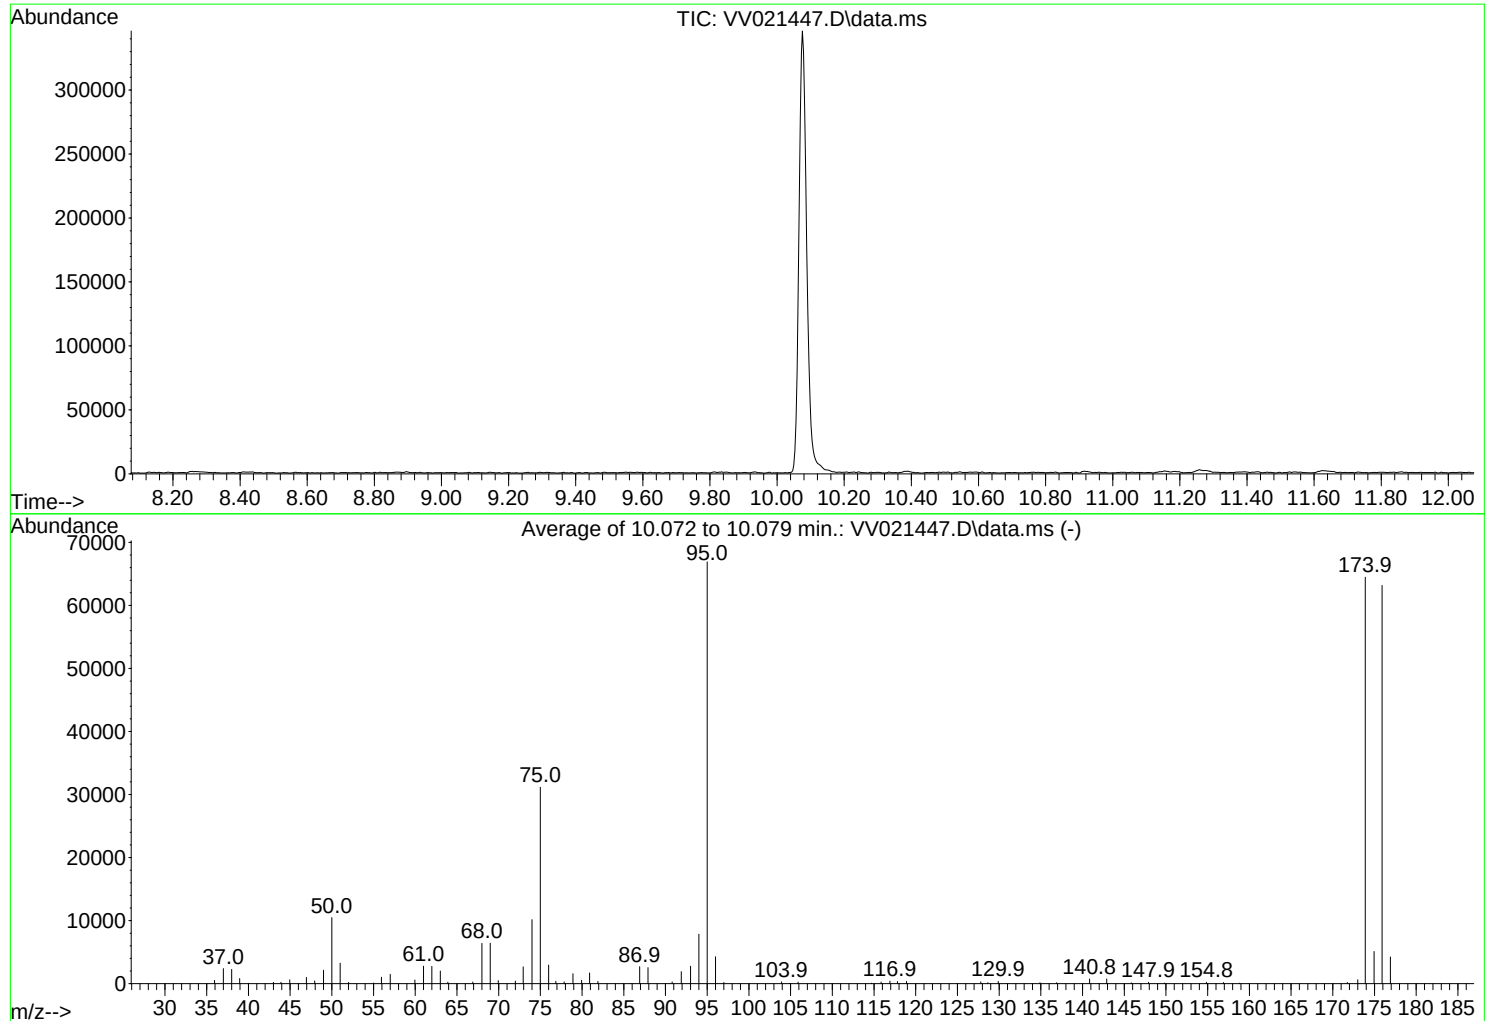

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.7	10473	PASS
75	95	30	80	46.6	31157	PASS
95	95	100	100	100.0	66912	PASS
96	95	5	9	6.4	4259	PASS
173	174	0.00	2	0.9	607	PASS
174	95	50	120	96.4	64477	PASS
175	174	5	9	7.9	5097	PASS
176	174	95	105	98.0	63173	PASS
177	176	5	10	6.7	4254	PASS

m/z	Abundance
36.00	494.0
37.00	2335.0
38.00	2354.0
39.00	1053.0
40.00	253.0
41.00	107.0
42.00	104.0
43.00	155.0
44.00	627.0
44.90	542.0
47.00	959.0
48.00	411.0
49.00	2195.0
50.00	10312.0
51.00	3355.0
52.00	233.0
55.00	223.0
55.90	987.0
57.00	1431.0
60.00	615.0
61.00	2970.0
62.00	2826.0
63.00	2052.0
63.90	214.0
66.90	272.0
68.00	6312.0
69.00	6431.0
70.00	490.0
72.00	402.0
73.00	2604.0
74.00	10049.0
75.00	30888.0
76.00	2958.0
76.80	388.0
77.90	333.0
78.90	1606.0
80.00	523.0
80.90	1761.0
81.90	375.0
86.90	2795.0
87.90	2468.0
90.80	265.0
91.90	1836.0
93.00	2691.0
94.00	7650.0
95.00	66424.0
96.00	4366.0
97.00	164.0
103.90	258.0
105.90	303.0
115.90	212.0
116.90	439.0
117.80	391.0
118.90	342.0
127.80	267.0
128.70	171.0
129.90	354.0
134.90	172.0
136.80	124.0
140.90	751.0
141.90	120.0
142.90	722.0
145.90	114.0
148.00	188.0
149.80	103.0
154.80	204.0
156.90	145.0
158.80	120.0
171.70	159.0
173.00	560.0
173.90	61856.0
175.00	4969.0
175.90	60840.0
176.90	4199.0

Instrument :
MSVOA_V
ClientSampleId :
BFB161

m/z	Abundance
38.80	137.0
40.00	185.0
41.00	118.0
42.00	134.0
43.90	361.0
55.00	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB161

m/z	Abundance
35.90	496.0
37.00	2418.0
38.00	2101.0
39.00	853.0
40.00	232.0
43.00	225.0
43.90	540.0
45.00	661.0
46.00	123.0
46.90	965.0
47.90	443.0
49.00	2015.0
50.00	10241.0
51.00	3025.0
52.00	178.0
55.00	242.0
56.00	978.0
57.00	1505.0
59.90	539.0
61.00	2520.0
62.00	2638.0
63.00	1889.0
63.90	230.0
66.90	224.0
68.00	6202.0
69.00	6186.0
69.90	474.0
72.00	400.0
72.90	2631.0
74.00	9890.0
75.00	30432.0
76.00	2817.0
76.90	392.0
77.80	232.0
78.90	1531.0
79.90	543.0
80.90	1577.0
81.90	335.0
85.80	104.0
86.90	2529.0
87.90	2552.0
90.80	256.0
91.90	1836.0
93.00	2793.0
94.00	7701.0
95.00	65248.0
96.00	4099.0
97.00	172.0
103.90	279.0
104.90	102.0
105.90	234.0
114.70	126.0
115.80	271.0
116.90	384.0
117.80	274.0
118.90	368.0
127.80	311.0
128.60	134.0
129.90	345.0
134.90	131.0
137.00	190.0
140.80	697.0
142.90	730.0
145.80	148.0
147.80	218.0
149.80	120.0
154.90	241.0
156.90	180.0
171.80	181.0
173.00	624.0
173.90	64856.0
174.90	5011.0
175.90	63320.0
176.90	4160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB161

m/z	Abundance
35.90	498.0
37.00	2442.0
38.00	2334.0
39.00	980.0
40.00	257.0
43.00	212.0
43.90	611.0
44.90	613.0
46.90	1055.0
48.00	453.0
49.00	2229.0
50.00	10865.0
51.00	3373.0
52.00	225.0
55.00	242.0
56.00	1068.0
57.00	1516.0
59.90	635.0
61.00	2801.0
62.00	2752.0
63.00	2054.0
63.90	243.0
66.90	256.0
68.00	6692.0
69.00	6681.0
70.00	486.0
72.00	422.0
72.90	2778.0
74.00	10502.0
75.00	32152.0
76.00	3100.0
76.90	381.0
77.80	290.0
78.90	1594.0
79.90	562.0
80.90	1753.0
81.90	399.0
86.90	2744.0
87.90	2564.0
90.80	285.0
91.90	2014.0
93.00	2860.0
94.00	8223.0
95.00	69064.0
96.00	4313.0
97.00	191.0
103.90	282.0
105.90	265.0
114.70	101.0
115.90	259.0
116.90	429.0
117.80	363.0
118.90	340.0
127.80	302.0
128.70	168.0
129.90	388.0
134.90	172.0
136.90	162.0
140.90	764.0
142.90	750.0
145.90	144.0
147.90	221.0
149.80	112.0
154.90	231.0
156.90	179.0
158.80	118.0
171.70	184.0
173.00	638.0
173.90	66720.0
174.90	5310.0
175.90	65360.0
176.90	4403.0

Instrument :
MSVOA_V
ClientSampleId :
BFB161