

Data File : VV011100.D
Acq On : 29 May 2019 12:01
Operator : SY/MD
Sample : K3006-12
Misc : 3.65G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFH74

Quant Time: May 30 03:55:13 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM052819S.M
Quant Title : VOC Analysis
QLast Update : Thu May 30 03:51:47 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	342166	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	291680	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	94872	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	122550	26.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.48%
7) Chloroethane-d5	1.56	69	97533	29.13	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	116.52%
10) 1,1-Dichloroethene-d2	1.88	63	161	0.02	ug/L	-0.24
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.08%#
20) 2-Butanone-d5	3.94	46	111568	69.00	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	138.00%#
24) Chloroform-d	4.40	84	225397	27.16	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	108.64%
26) 1,2-Dichloroethane-d4	5.08	65	158062	29.79	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	119.16%
29) Benzene-d6	5.09	84	510473	29.89	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	119.56%
33) 1,2-Dichloropropane-d6	6.12	67	167656	30.85	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	123.40%#
37) Toluene-d8	7.36	98	438568	27.86	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	111.44%
38) trans-1,3-Dichloropropene-	7.66	79	68071	26.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	107.56%
39) 2-Hexanone-d5	8.13	63	84454	71.34	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	142.68%#
48) 1,1,2,2-Tetrachloroethane-	10.26	84	142291	30.46	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	121.84%#
61) 1,2-Dichlorobenzene-d4	11.67	152	103182	27.50	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	110.00%


Target Compounds					Qvalue
13) Acetone	2.19	43	8013	4.375 ug/L	99
25) Chloroform	4.42	83	19460	2.017 ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV011100.D
Acq On : 29 May 2019 12:01
Operator : SY/MD
Sample : K3006-12
Misc : 3.65G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFH74

Quant Time: May 30 03:55:13 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM052819S.M
Quant Title : VOC Analysis
QLast Update : Thu May 30 03:51:47 2019
Response via : Initial Calibration

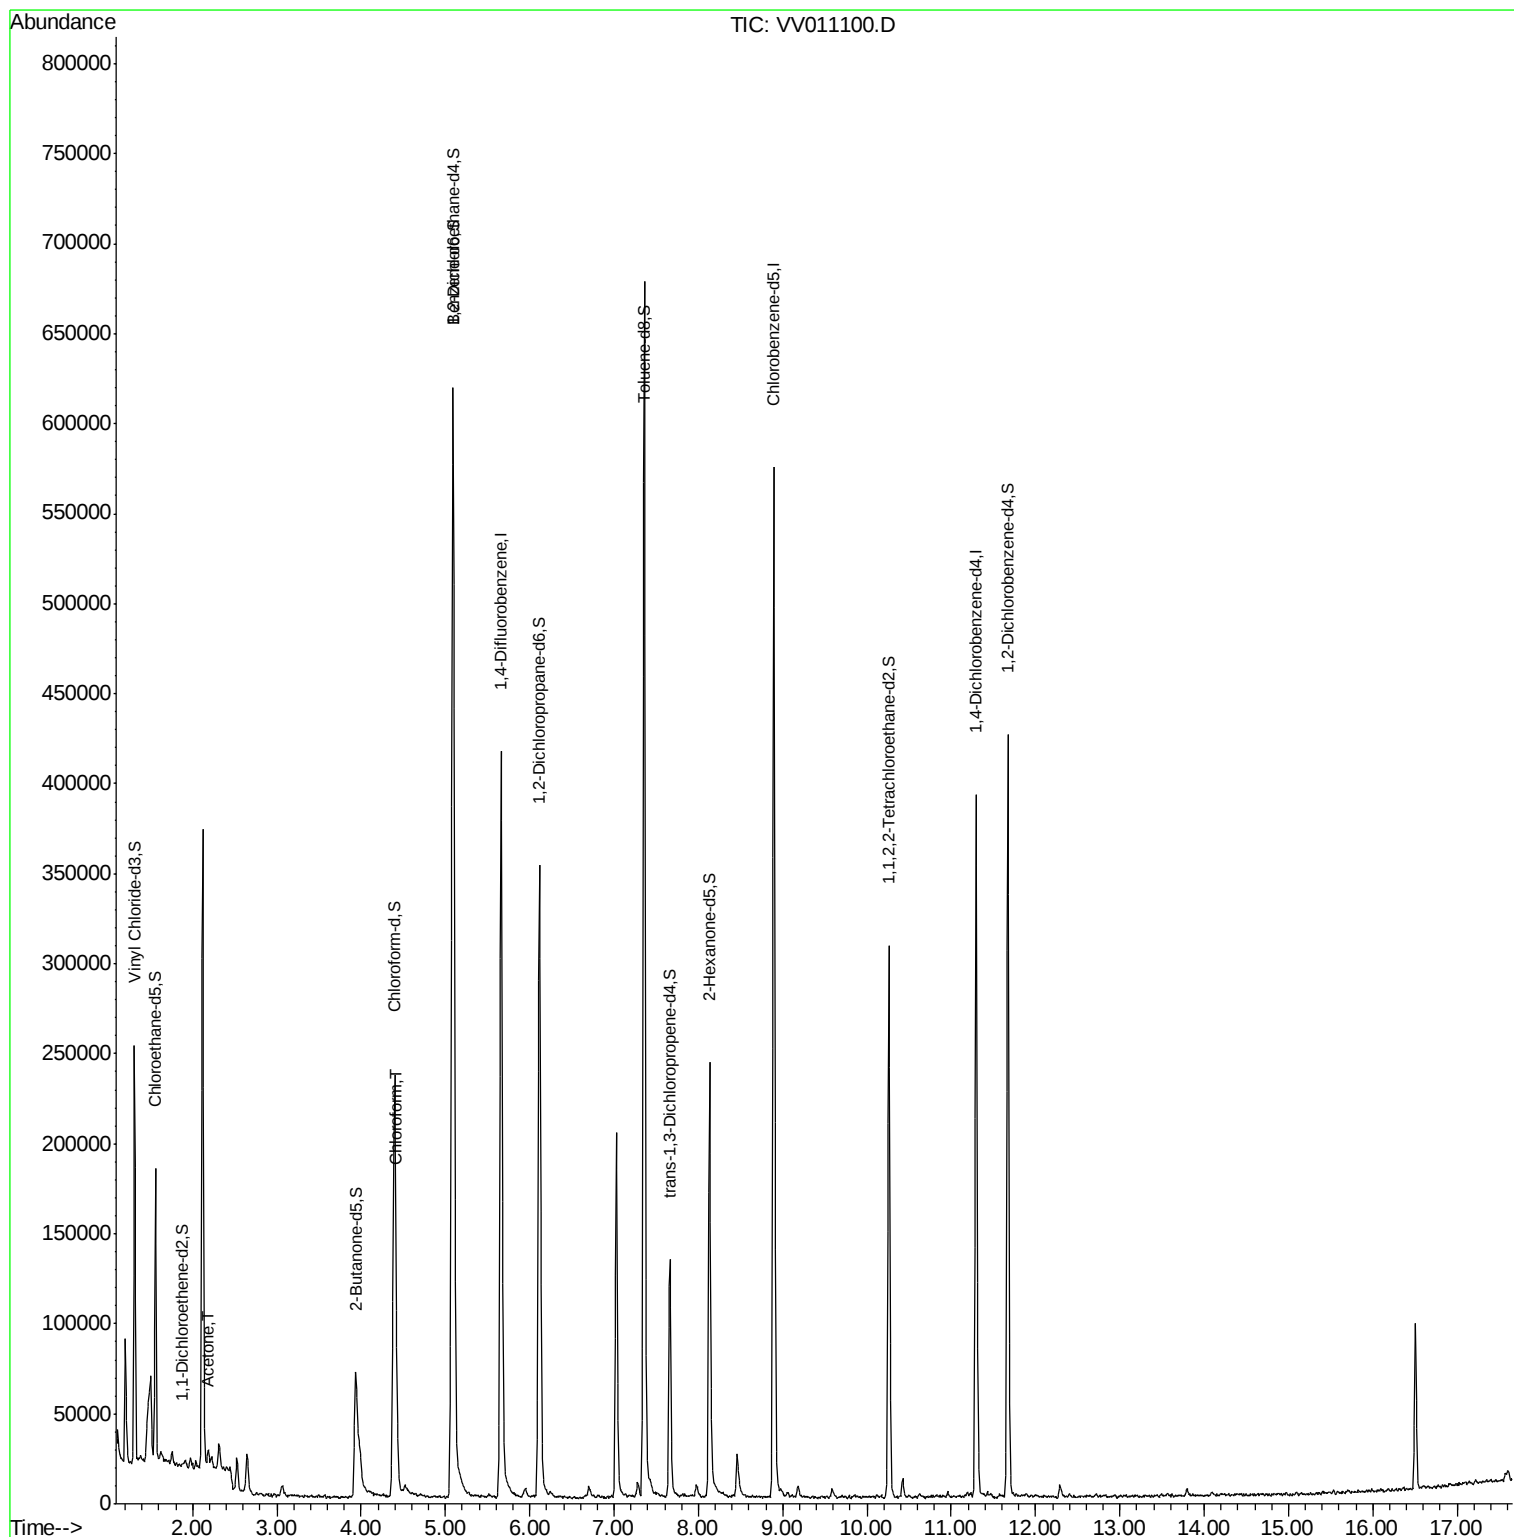

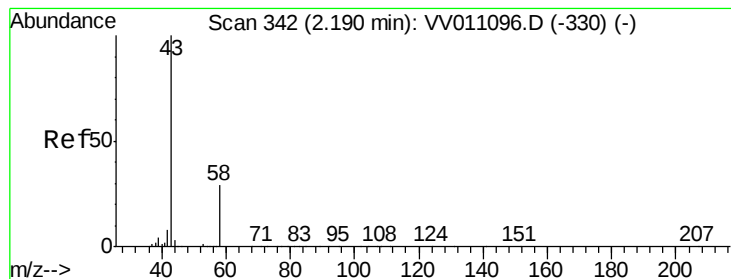

#13

Acetone

Concen: 4.375 ug/L

RT: 2.19 min Scan# 341

Delta R.T. -0.00 min

Lab File: VV011100.D

Acq: 29 May 2019 12:01

Instrument :

MSVOA_V

ClientSampleId :


BFH74

Tgt Ion: 43 Resp: 8013

Ion Ratio Lower Upper

43 100

58 27.0 0.0 54.8

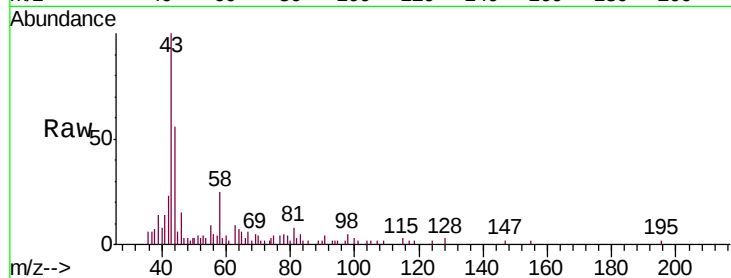

Abundance Ion 43.00 (42.70 to 43.70): VV011096.D (-330) (-)

Ion 58.00 (57.70 to 58.70): VV011096.D (-330) (-)

2.19

6000



4000

2000

0

Time-->

2.15 2.20

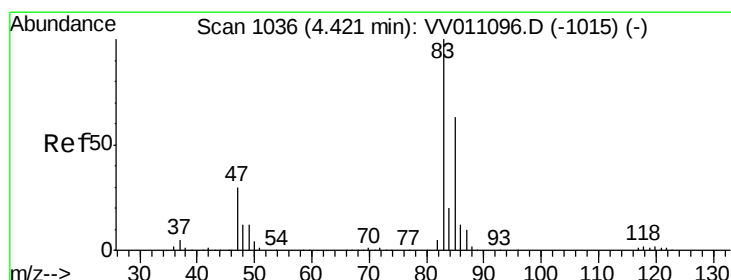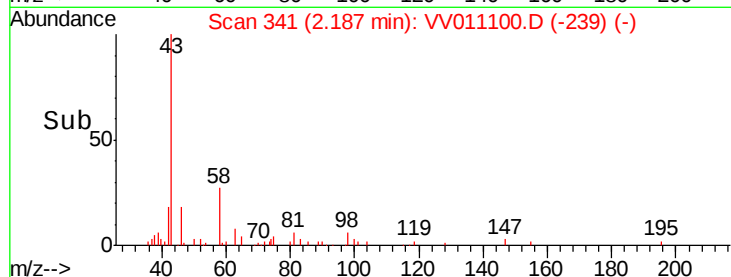

#25

Chloroform

Concen: 2.017 ug/L

RT: 4.42 min Scan# 1036

Delta R.T. 0.00 min

Lab File: VV011100.D


Acq: 29 May 2019 12:01

Tgt Ion: 83 Resp: 19460

Ion Ratio Lower Upper

83 100

85 77.3 46.2 85.8

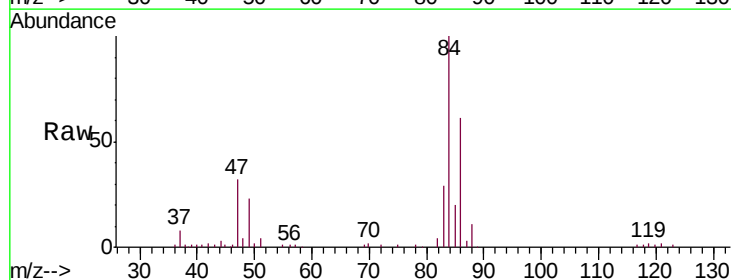

Abundance Ion 83.00 (82.70 to 83.70): VV011096.D (-1015) (-)

Ion 85.00 (84.70 to 85.70): VV011096.D (-1015) (-)

4.42

8000

6000

4000

2000

0

Time-->

4.35 4.40 4.45 4.50

