

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052919\
 Data File : VV011098.D
 Acq On : 29 May 2019 11:05
 Operator : SY/MD
 Sample : K3006-10
 Misc : 4.53G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFH78

Quant Time: May 30 04:02:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM052819S.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 30 03:51:47 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	404157	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	357417	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	144927	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	132482	23.91	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.64%
7) Chloroethane-d5	1.57	69	101448	25.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.60%
10) 1,1-Dichloroethene-d2	2.12	63	203294	19.72	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	78.88%
20) 2-Butanone-d5	3.94	46	74271	38.89	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.78%
24) Chloroform-d	4.40	84	207729	21.19	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.76%
26) 1,2-Dichloroethane-d4	5.08	65	139771	22.31	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.24%
29) Benzene-d6	5.09	84	519045	24.80	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.20%
33) 1,2-Dichloropropane-d6	6.11	67	160568	24.12	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.48%
37) Toluene-d8	7.36	98	476476	24.70	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.80%
38) trans-1,3-Dichloropropene-	7.66	79	66384	21.40	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.60%
39) 2-Hexanone-d5	8.13	63	56641	39.05	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.10%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	115993	20.26	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.04%
61) 1,2-Dichlorobenzene-d4	11.67	152	133175	23.24	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.96%


Target Compounds					Ovalue
13) Acetone	2.19	43	9938	4.593 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052919\
Data File : VV011098.D
Acq On : 29 May 2019 11:05
Operator : SY/MD
Sample : K3006-10
Misc : 4.53G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFH78

Quant Time: May 30 04:02:17 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM052819S.M
Quant Title : VOC Analysis
QLast Update : Thu May 30 03:51:47 2019
Response via : Initial Calibration

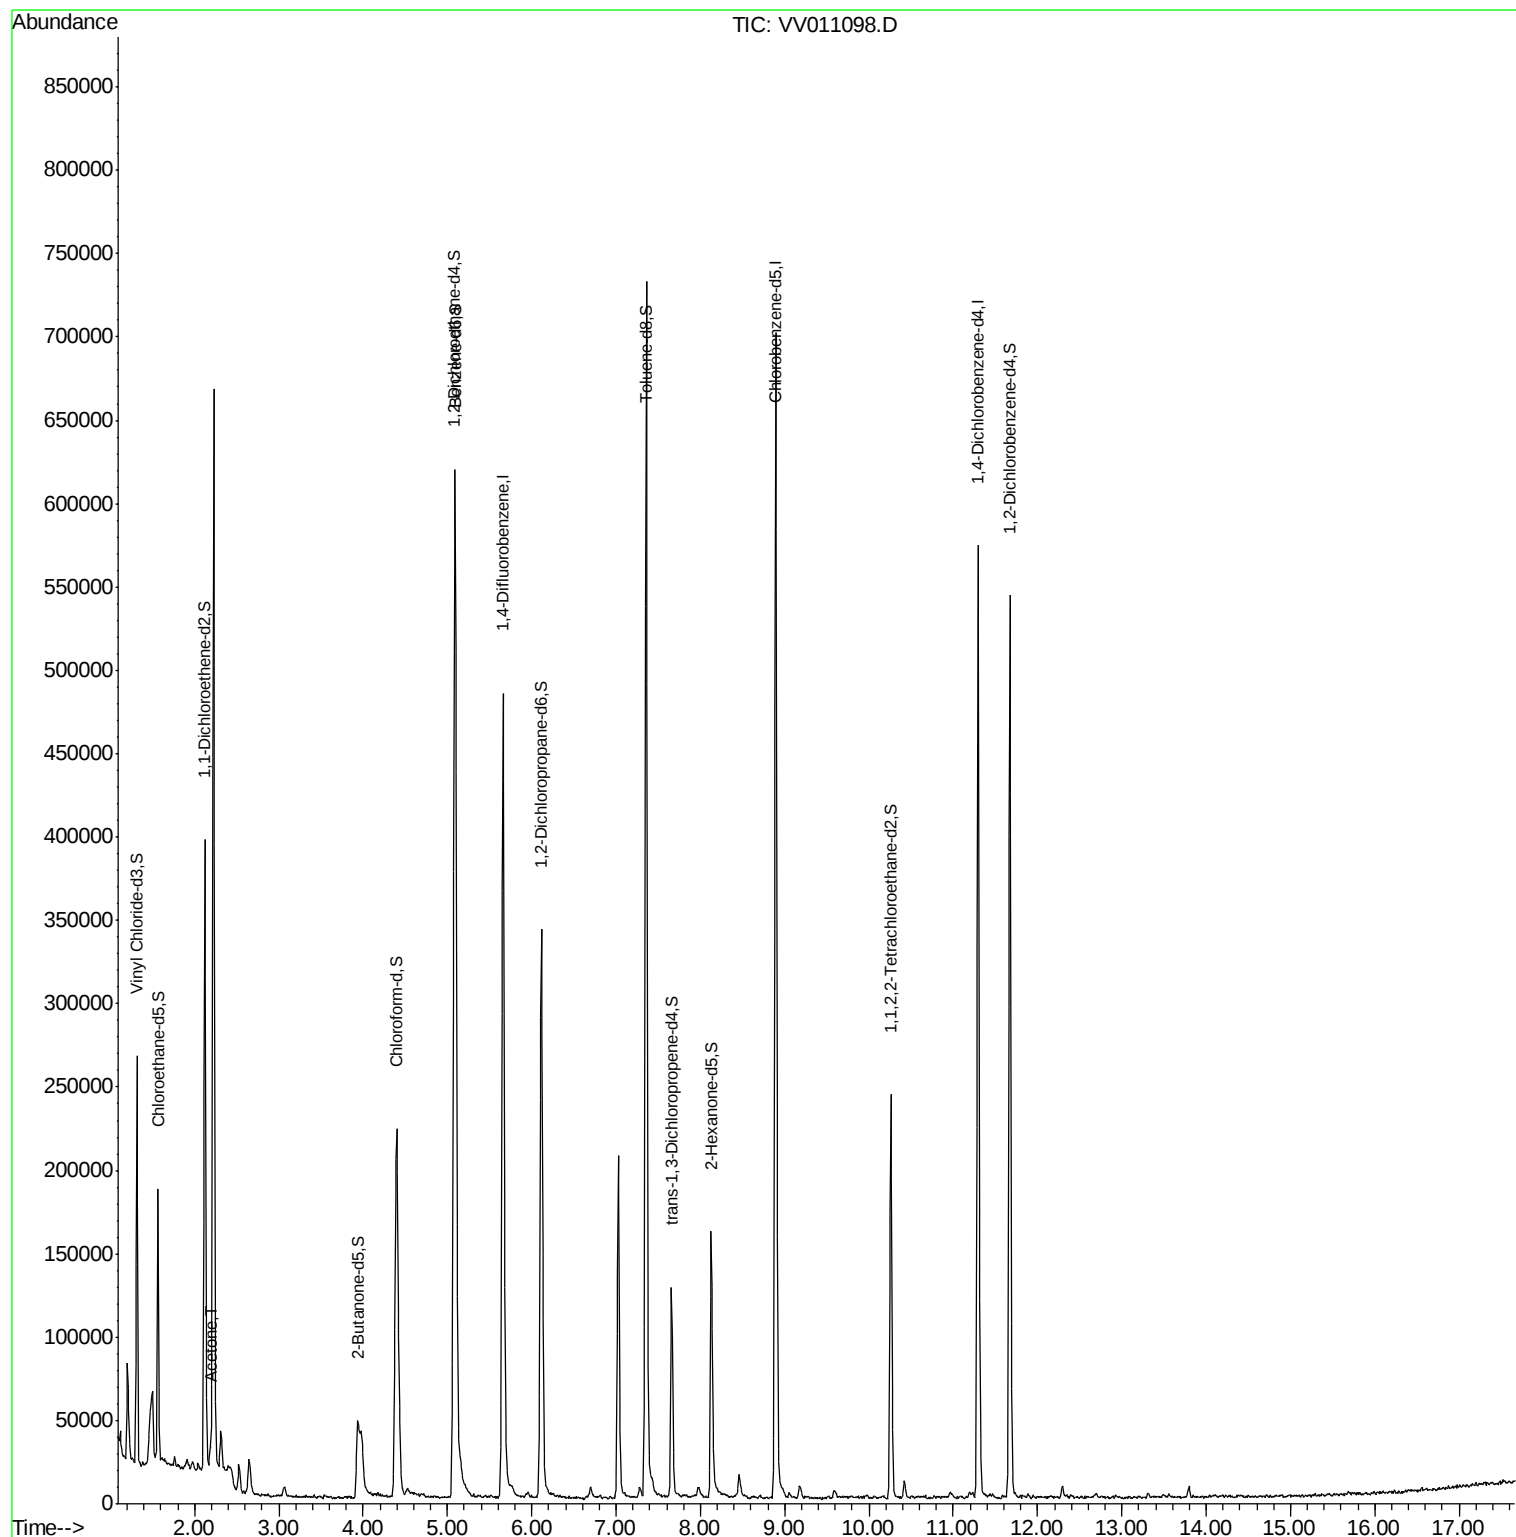

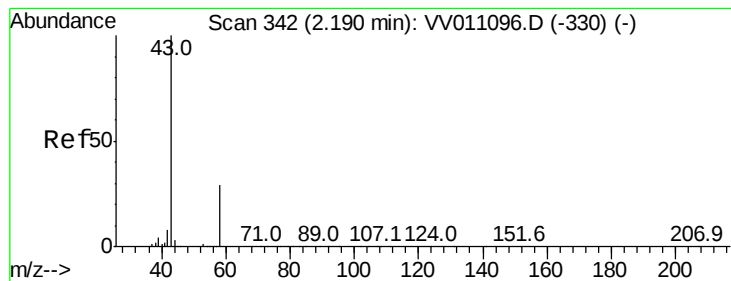

#13

Acetone

Concen: 4.593 ug/L

RT: 2.19 min Scan# 341

Delta R.T. -0.00 min

Lab File: VV011098.D

Acq: 29 May 2019 11:05

Instrument :
MSVOA_V
ClientSampleId :
BFH78

Tot Ion: 43 Resp: 9938

Ion Ratio Lower Upper

43 100

58 21.0 0.0 54.8

