

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV052919\
 Data File : VV011104.D
 Acq On : 29 May 2019 13:54
 Operator : SY/MD
 Sample : K3006-16
 Misc : 4.45G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFH82

Quant Time: May 30 04:14:26 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM052819S.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 30 03:51:47 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	252332	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	236379	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	93764	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	72741	21.03	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.12%
7) Chloroethane-d5	1.57	69	61164	24.77	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.08%
10) 1,1-Dichloroethene-d2	2.12	63	114662	17.82	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.28%
20) 2-Butanone-d5	3.94	46	65022	54.53	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.06%
24) Chloroform-d	4.40	84	147591	24.12	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.48%
26) 1,2-Dichloroethane-d4	5.08	65	103415	26.43	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.72%
29) Benzene-d6	5.10	84	327489	23.66	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.64%
33) 1,2-Dichloropropane-d6	6.12	67	108423	24.62	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.48%
37) Toluene-d8	7.36	98	296416	23.23	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.92%
38) trans-1,3-Dichloropropene-	7.66	79	41983	20.46	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.84%
39) 2-Hexanone-d5	8.13	63	47333	49.34	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.68%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	96040	25.36	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.44%
61) 1,2-Dichlorobenzene-d4	11.67	152	91263	24.61	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.44%


Target Compounds					Ovalue
13) Acetone	2.19	43	7319	5.418 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV052919\
Data File : VV011104.D
Acq On : 29 May 2019 13:54
Operator : SY/MD
Sample : K3006-16
Misc : 4.45G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFH82

Quant Time: May 30 04:14:26 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM052819S.M
Quant Title : VOC Analysis
QLast Update : Thu May 30 03:51:47 2019
Response via : Initial Calibration

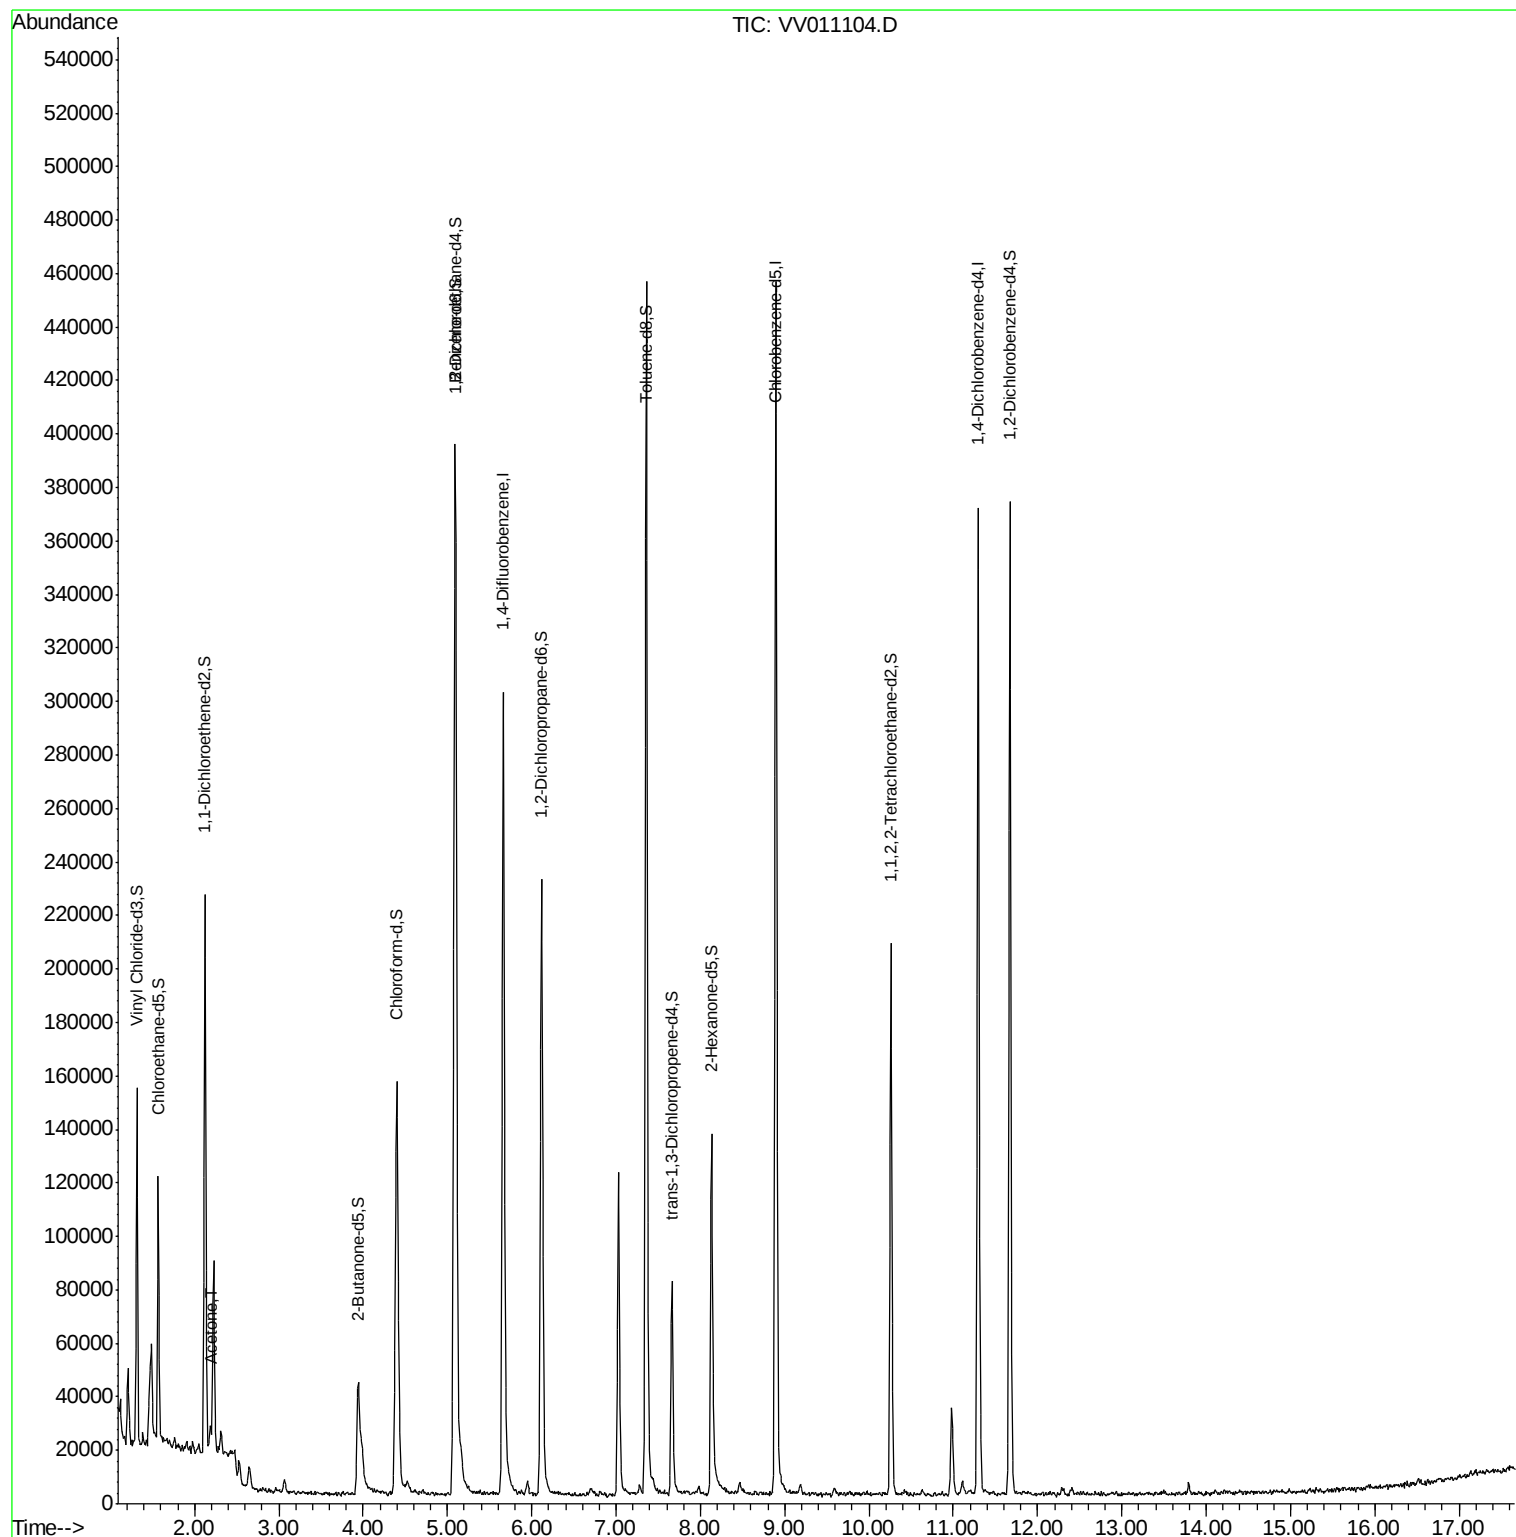

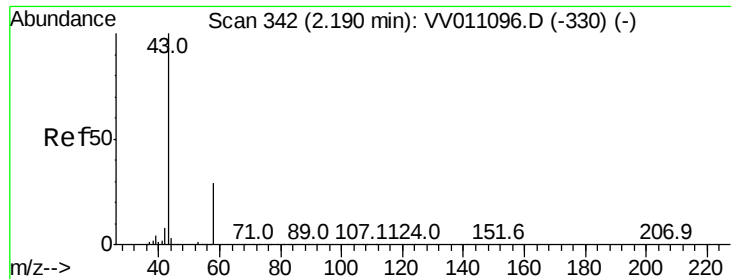

#13
 Acetone
 Concen: 5.418 ug/L
 RT: 2.19 min Scan# 342
 Delta R.T. -0.00 min
 Lab File: VV011104.D
 Acq: 29 May 2019 13:54

Instrument :
 MSVOA_V
 ClientSampleId :
 BFH82

Tot Ion: 43 Resp: 7319
 Ion Ratio Lower Upper
 43 100
 58 26.7 0.0 54.8

