


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV052919\
 Data File : VV011095.D
 Acq On : 29 May 2019 08:58
 Operator : SY/MD
 Sample : BFB65
 Misc : 5.00G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB65

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM052819S.M
 Title : VOC Analysis
 Last Update : Thu May 30 04:49:33 2019

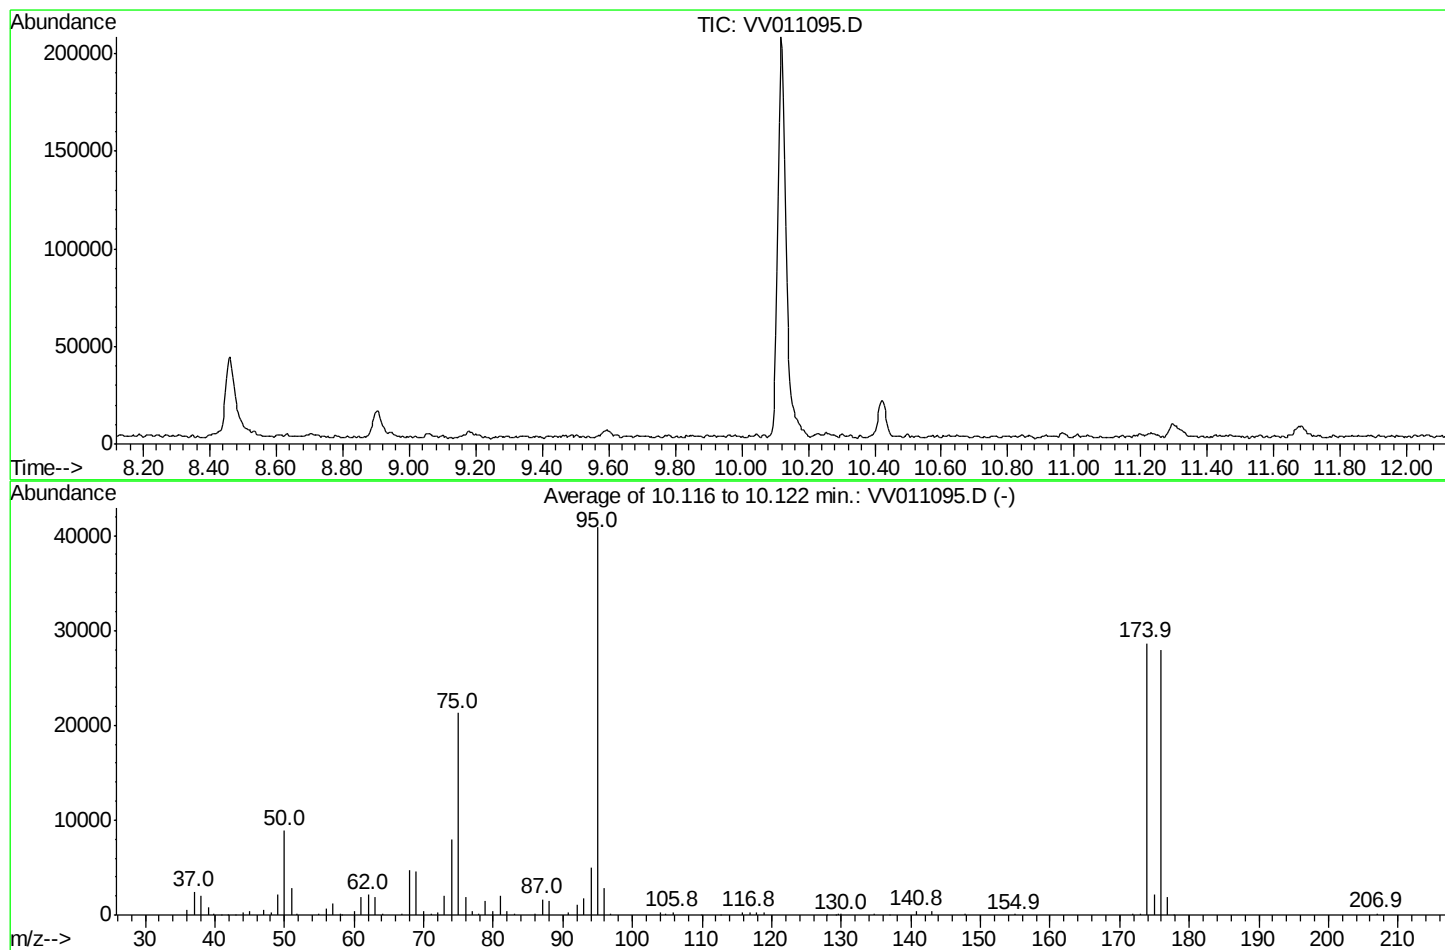

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	8900	PASS
75	95	30	80	52.1	21279	PASS
95	95	100	100	100.0	40877	PASS
96	95	5	9	7.0	2846	PASS
173	174	0.00	2	0.6	172	PASS
174	95	50	120	70.1	28650	PASS
175	174	5	9	7.7	2195	PASS
176	174	95	101	97.7	27994	PASS
177	176	5	9	6.9	1922	PASS

m/z	Abundance
38.00	130.0
39.10	204.0
39.90	264.0
41.00	249.0
42.20	199.0
43.00	251.0
44.00	765.0
45.10	143.0
48.10	107.0
50.70	106.0
51.80	103.0
52.80	118.0
55.00	137.0
56.20	141.0
57.00	105.0
66.00	115.0
67.00	147.0
68.80	149.0
74.90	126.0
128.00	102.0
168.80	164.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
35.90	566.0
37.00	2508.0
38.00	2213.0
39.00	901.0
39.90	411.0
41.00	291.0
42.10	116.0
43.00	242.0
44.00	900.0
45.00	500.0
47.00	698.0
48.00	424.0
49.00	2132.0
50.00	8476.0
51.00	2793.0
51.90	187.0
54.90	285.0
56.00	889.0
57.00	1290.0
58.00	107.0
60.00	385.0
61.00	1911.0
62.00	2188.0
63.00	1821.0
64.10	150.0
66.90	258.0
68.00	4651.0
69.00	4740.0
70.00	485.0
72.00	248.0
73.00	1984.0
74.00	7706.0
75.00	20904.0
76.00	1949.0
77.10	352.0
77.80	189.0
78.90	1388.0
80.00	514.0
81.00	2004.0
81.90	343.0
83.10	137.0
85.90	127.0
87.00	1456.0
88.00	1482.0
90.80	223.0
92.10	1160.0
93.00	1704.0
94.00	5054.0
95.00	39160.0
96.00	2867.0
96.90	142.0
104.00	268.0
104.80	142.0
105.80	286.0
109.90	107.0
115.80	220.0
116.80	318.0
117.80	181.0
118.90	298.0
127.90	167.0
129.70	112.0
130.10	146.0
134.80	103.0
140.90	453.0
142.90	439.0
147.80	150.0
168.90	113.0
171.80	110.0
173.90	26752.0
174.90	2212.0
175.90	26256.0
176.90	1834.0
206.90	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
35.90	582.0
37.00	2526.0
38.00	2284.0
39.00	1050.0
39.90	320.0
41.00	314.0
42.20	131.0
43.00	258.0
44.00	982.0
44.90	533.0
47.00	592.0
48.00	425.0
49.00	2239.0
50.00	9182.0
51.00	2950.0
51.90	198.0
55.00	332.0
56.00	799.0
57.00	1337.0
58.00	112.0
60.10	353.0
61.00	1997.0
62.00	2250.0
63.00	2041.0
64.00	153.0
66.80	282.0
68.00	4903.0
69.00	5009.0
70.00	458.0
71.00	119.0
72.00	246.0
73.00	2087.0
74.00	8103.0
75.00	22136.0
76.00	1969.0
77.10	394.0
77.80	188.0
78.90	1548.0
79.90	467.0
81.00	2036.0
81.90	393.0
83.10	145.0
85.90	144.0
87.00	1667.0
88.00	1591.0
90.80	277.0
92.10	1094.0
93.00	1772.0
94.00	5178.0
95.00	42336.0
96.00	2969.0
96.80	142.0
104.00	304.0
104.80	135.0
105.80	300.0
115.80	225.0
116.90	342.0
117.80	244.0
118.90	293.0
127.90	160.0
129.50	130.0
130.00	105.0
134.80	158.0
136.90	115.0
140.90	451.0
142.90	447.0
147.80	155.0
155.00	117.0
168.80	157.0
171.80	118.0
173.90	29664.0
174.90	2271.0
175.90	28872.0
176.90	1955.0
177.80	105.0
207.00	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
35.90	586.0
37.00	2348.0
38.00	2077.0
39.00	1096.0
39.90	290.0
40.90	291.0
41.90	122.0
43.00	264.0
44.00	1106.0
44.90	518.0
47.00	470.0
48.10	417.0
49.00	2125.0
50.00	9044.0
51.00	2739.0
52.00	189.0
55.00	330.0
56.00	728.0
57.00	1272.0
58.20	121.0
60.10	316.0
61.00	1844.0
62.00	1980.0
63.00	1878.0
64.00	179.0
66.80	289.0
68.00	4527.0
69.00	4632.0
70.00	431.0
71.00	144.0
71.90	238.0
73.00	1958.0
74.00	7933.0
75.00	21176.0
76.00	1812.0
77.00	362.0
77.90	183.0
78.90	1554.0
79.90	378.0
80.90	1856.0
81.90	405.0
83.00	137.0
85.90	154.0
87.00	1804.0
87.90	1530.0
90.90	295.0
92.00	979.0
93.00	1710.0
94.00	4748.0
95.00	41136.0
96.00	2702.0
96.80	157.0
104.00	277.0
105.80	270.0
112.70	131.0
115.80	199.0
116.90	349.0
117.80	254.0
118.90	289.0
127.90	161.0
129.20	148.0
129.90	114.0
134.80	149.0
140.80	463.0
143.00	432.0
147.80	141.0
154.90	113.0
168.70	163.0
171.80	105.0
172.90	518.0
173.90	29536.0
175.00	2102.0
175.90	28856.0
176.90	1978.0
207.00	140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65