


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV052920\
 Data File : VV016313.D
 Acq On : 29 May 2020 11:28
 Operator : SY/MD
 Sample : BFB34
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB34

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR052620WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Jun 01 00:52:43 2020

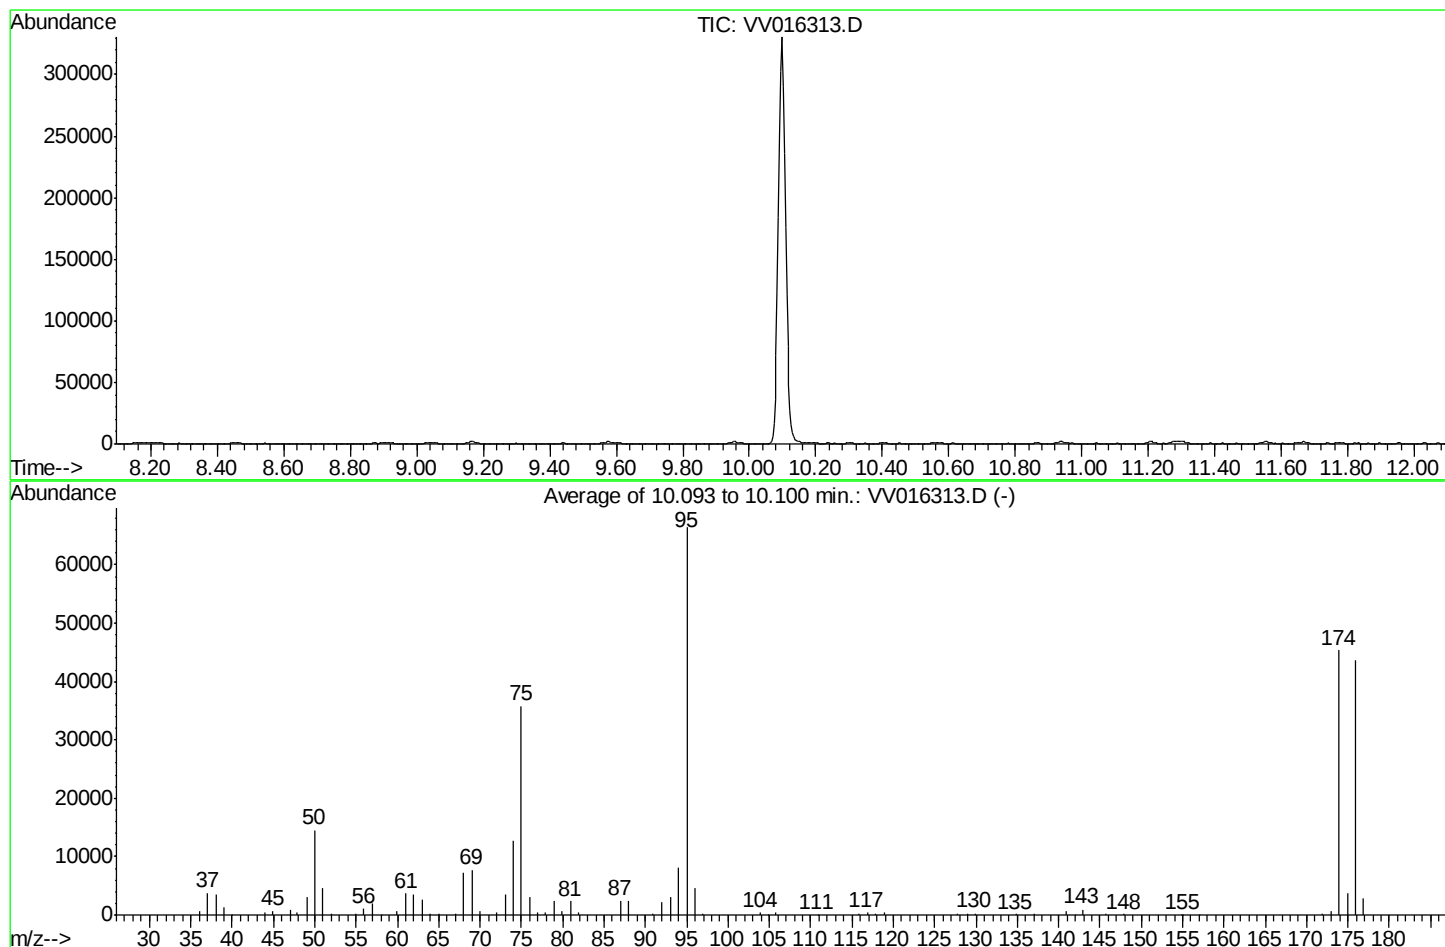

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	14512	PASS
75	95	30	80	54.0	35850	PASS
95	95	100	100	100.0	66416	PASS
96	95	5	9	7.0	4633	PASS
173	174	0.00	2	1.5	663	PASS
174	95	50	120	68.3	45346	PASS
175	174	5	9	8.2	3731	PASS
176	174	95	101	96.3	43682	PASS
177	176	5	9	6.8	2958	PASS

m/z	Abundance
36.00	738.0
37.00	3797.0
38.00	3432.0
39.00	1306.0
40.00	235.0
44.00	701.0
44.90	657.0
47.10	850.0
47.90	500.0
49.00	3202.0
50.00	14010.0
51.00	4499.0
52.00	288.0
54.90	192.0
56.00	1006.0
57.00	1942.0
60.00	648.0
61.00	3416.0
62.00	3545.0
63.00	2439.0
64.00	270.0
65.00	227.0
67.10	232.0
68.00	7191.0
69.00	7480.0
69.90	586.0
72.00	395.0
73.00	3252.0
74.00	12378.0
75.00	33968.0
76.00	3047.0
76.90	349.0
78.00	336.0
78.90	2386.0
79.90	589.0
80.90	2336.0
81.90	416.0
87.00	2360.0
87.90	2206.0
91.00	249.0
92.00	1977.0
93.00	2704.0
94.00	7682.0
95.00	62888.0
96.00	4442.0
96.90	138.0
103.90	406.0
104.90	117.0
105.80	308.0
115.80	220.0
116.80	367.0
117.90	290.0
118.90	376.0
127.80	268.0
128.90	130.0
129.80	292.0
134.80	176.0
137.00	133.0
140.90	614.0
142.10	103.0
142.90	846.0
145.70	122.0
147.90	120.0
154.80	150.0
172.00	304.0
173.00	681.0
173.90	42008.0
174.90	3541.0
175.90	40232.0
176.90	2853.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

m/z	Abundance
36.00	829.0
37.00	3973.0
38.00	3653.0
39.00	1350.0
40.00	210.0
44.00	758.0
44.90	699.0
47.10	957.0
47.90	526.0
49.00	3296.0
50.00	15097.0
51.00	4803.0
52.00	280.0
54.90	227.0
55.90	1126.0
57.00	2088.0
60.00	656.0
61.00	3840.0
62.00	3691.0
63.00	2682.0
64.00	331.0
65.00	221.0
67.00	214.0
68.00	7548.0
69.00	8112.0
69.90	641.0
72.00	424.0
73.00	3535.0
74.00	13208.0
75.00	37000.0
76.00	3202.0
76.90	372.0
77.90	373.0
78.90	2525.0
79.90	668.0
80.90	2494.0
81.90	474.0
87.00	2549.0
87.90	2571.0
90.90	285.0
92.00	2161.0
93.00	3092.0
94.00	8419.0
95.00	68672.0
96.00	4827.0
96.90	146.0
103.90	373.0
104.90	119.0
105.80	376.0
110.80	114.0
115.80	224.0
116.90	451.0
117.90	326.0
118.90	433.0
127.80	252.0
129.00	164.0
129.90	314.0
134.80	189.0
137.00	147.0
140.90	668.0
142.00	107.0
142.90	940.0
145.70	152.0
147.90	171.0
155.00	164.0
171.90	302.0
172.90	680.0
173.90	46848.0
174.90	3932.0
175.90	45240.0
176.90	3078.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

m/z	Abundance
36.00	757.0
37.00	3755.0
38.00	3448.0
39.00	1313.0
40.00	191.0
44.00	760.0
45.00	655.0
47.00	954.0
47.90	491.0
49.00	2987.0
50.00	14431.0
51.00	4627.0
52.00	228.0
54.90	229.0
55.90	1140.0
57.00	2030.0
58.00	107.0
59.90	639.0
61.00	3837.0
62.00	3528.0
63.00	2635.0
64.00	315.0
64.90	168.0
67.00	194.0
68.00	7182.0
69.00	7740.0
69.90	595.0
72.00	440.0
73.00	3500.0
74.00	12715.0
75.00	36584.0
76.00	3154.0
77.00	375.0
77.90	364.0
78.90	2383.0
79.90	630.0
80.90	2376.0
81.90	510.0
86.90	2573.0
87.90	2539.0
90.90	322.0
92.00	2164.0
93.00	3126.0
94.00	8392.0
95.00	67688.0
96.00	4630.0
96.90	117.0
103.90	349.0
104.80	116.0
105.80	381.0
110.80	117.0
115.80	232.0
116.90	472.0
117.90	317.0
118.90	452.0
127.80	232.0
129.00	158.0
129.90	301.0
134.80	166.0
137.00	126.0
140.90	717.0
141.90	107.0
142.90	940.0
145.80	139.0
147.90	197.0
155.00	166.0
157.00	110.0
171.80	262.0
173.00	629.0
173.90	47184.0
174.90	3721.0
175.90	45576.0
176.90	2943.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

Scan 2788 (10.055 min): VV016313.D
BFB34

m/z	Abundance
39.90	206.0
43.90	216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34