

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV053019\
 Data File : VV011167.D
 Acq On : 31 May 2019 07:33
 Operator : SY/MD
 Sample : K3017-15RE
 Misc : 5.94G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A51E8RE

Manual Integrations
 APPROVED

MMDadoda
 6/11/2019 9:40:27 AM

Quant Time: May 31 09:05:41 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM053019S.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 31 08:21:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	334318	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	271746	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	79824	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	91674	20.27	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.08%
7) Chloroethane-d5	1.57	69	81315	23.38	ug/L	0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.52%
10) 1,1-Dichloroethene-d2	2.12	63	146597m	15.79	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.16%
20) 2-Butanone-d5	3.93	46	72483	43.84	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.68%
24) Chloroform-d	4.39	84	205033	25.09	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.36%
26) 1,2-Dichloroethane-d4	5.08	65	127293	23.90	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.60%
29) Benzene-d6	5.09	84	419383	28.42	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	113.68%
33) 1,2-Dichloropropane-d6	6.11	67	137818	29.15	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	116.60%
37) Toluene-d8	7.36	98	356491	25.60	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	102.40%
38) trans-1,3-Dichloropropene-	7.66	79	47387	22.15	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.60%
39) 2-Hexanone-d5	8.13	63	54583	50.79	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.58%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	98318	23.07	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.28%
61) 1,2-Dichlorobenzene-d4	11.67	152	70883	23.73	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.92%

Target Compounds					Ovalue
13) Acetone	2.18	43	129531	67.348	ug/L 100
15) Methyl Acetate	2.45	43	58576	20.240	ug/L 96
21) 2-Butanone	4.02	43	13229	5.863	ug/L 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV053019\
Data File : VV011167.D
Acq On : 31 May 2019 07:33
Operator : SY/MD
Sample : K3017-15RE
Misc : 5.94G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
A51E8RE

Manual Integrations
APPROVED

MMDadoda
6/11/2019 9:40:27 AM

Quant Time: May 31 09:05:41 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM053019S.M
Quant Title : VOC Analysis
QLast Update : Fri May 31 08:21:18 2019
Response via : Initial Calibration

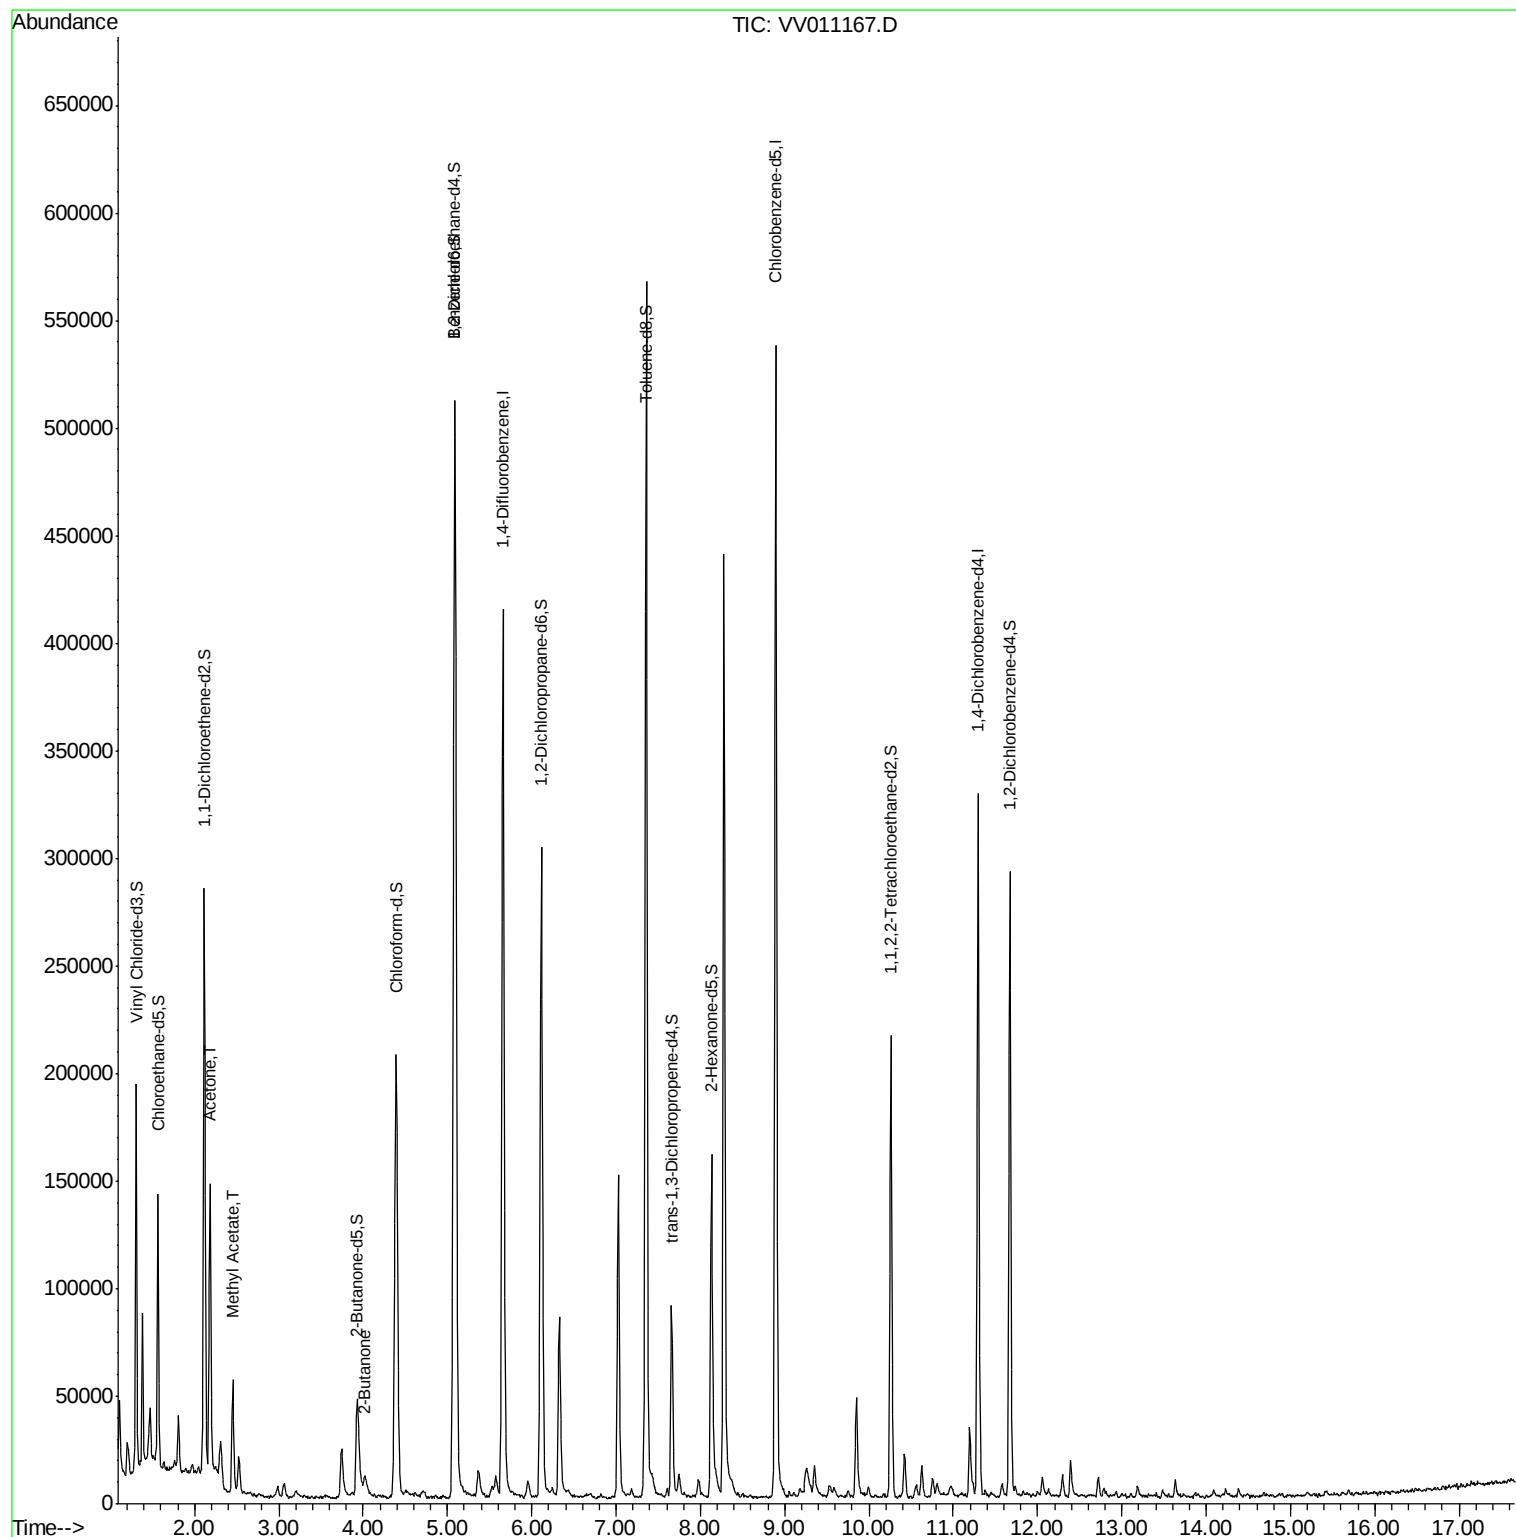

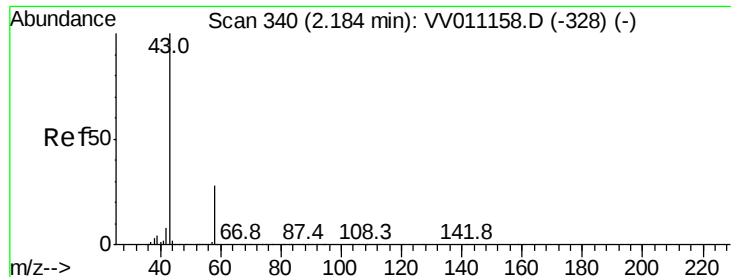

#13

Acetone

Concen: 67.348 ug/L

RT: 2.18 min Scan# 340

Delta R.T. -0.00 min

Lab File: VV011167.D

Acq: 31 May 2019 07:33

Instrument :

MSVOA_V

ClientSampleId :

A51E8RE

Tot Ion: 43 Resp: 129531

Ion Ratio Lower Upper

43 100





58 27.0 0.0 53.8

Manual Integrations

APPROVED

MMDadoda

6/11/2019 9:40:27 AM

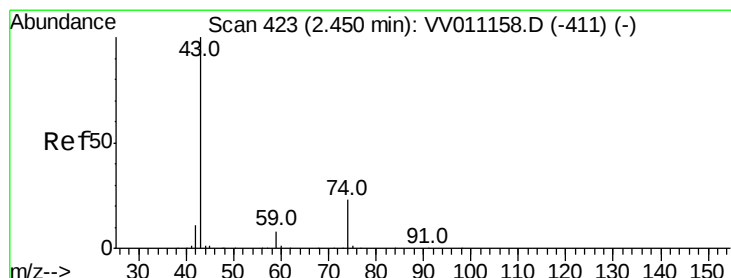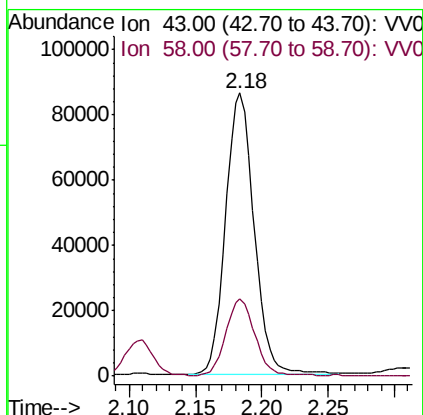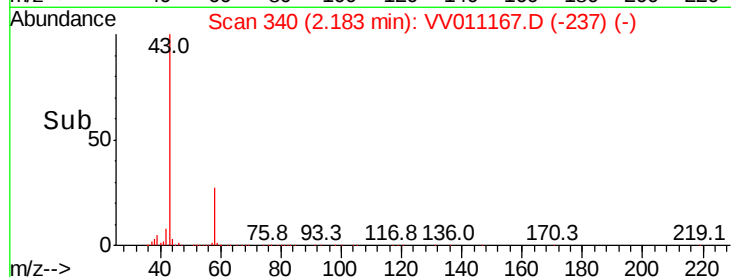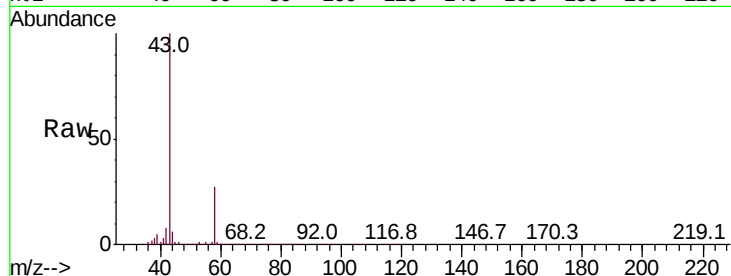

#15

Methyl Acetate

Concen: 20.240 ug/L

RT: 2.45 min Scan# 424

Delta R.T. 0.00 min

Lab File: VV011167.D




Acq: 31 May 2019 07:33


Tgt Ion: 43 Resp: 58576

Ion Ratio Lower Upper

43 100

74 22.0 16.2 24.4

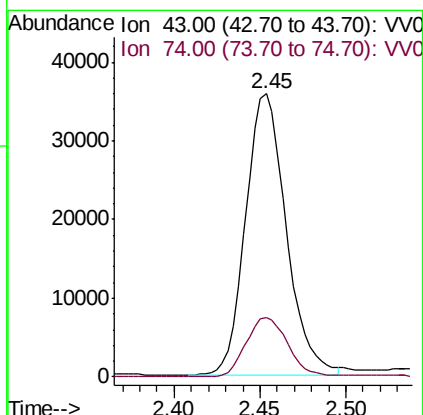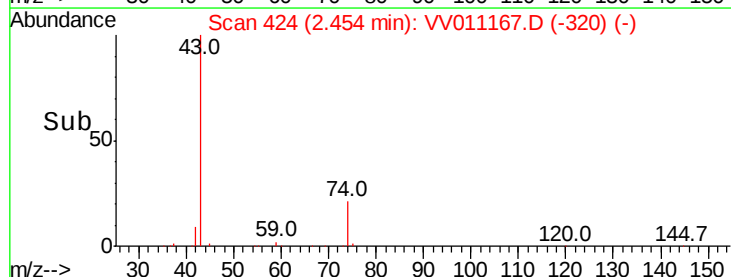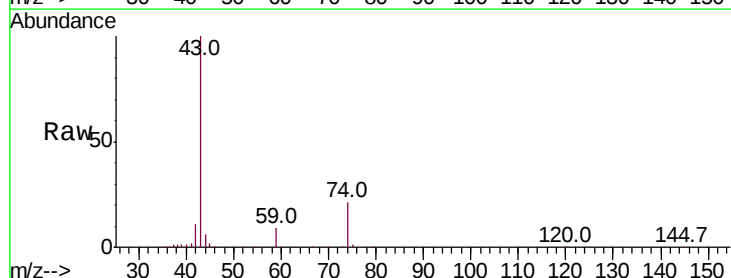

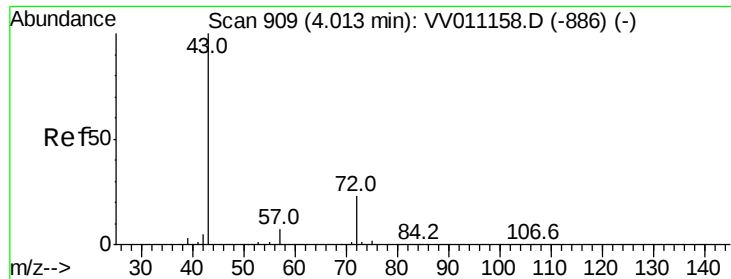

#21
 2-Butanone
 Concen: 5.863 ug/L
 RT: 4.02 min Scan# 912
 Delta R.T. 0.01 min
 Lab File: VV011167.D
 Acq: 31 May 2019 07:33

Instrument :
 MSVOA_V
 ClientSampleId :
 A51E8RE

Tot Ion	Ratio	Lower	Upper
43	100		
72	25.6	11.1	33.3

Manual Integrations
 APPROVED

MMDadoda
 6/11/2019 9:40:27 AM

