


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053019\
 Data File : VV011130.D
 Acq On : 30 May 2019 10:34
 Operator : SY/MD
 Sample : BFB66
 Misc : 5.00G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB66

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM053019S.M
 Title : VOC Analysis
 Last Update : Thu May 30 12:53:05 2019

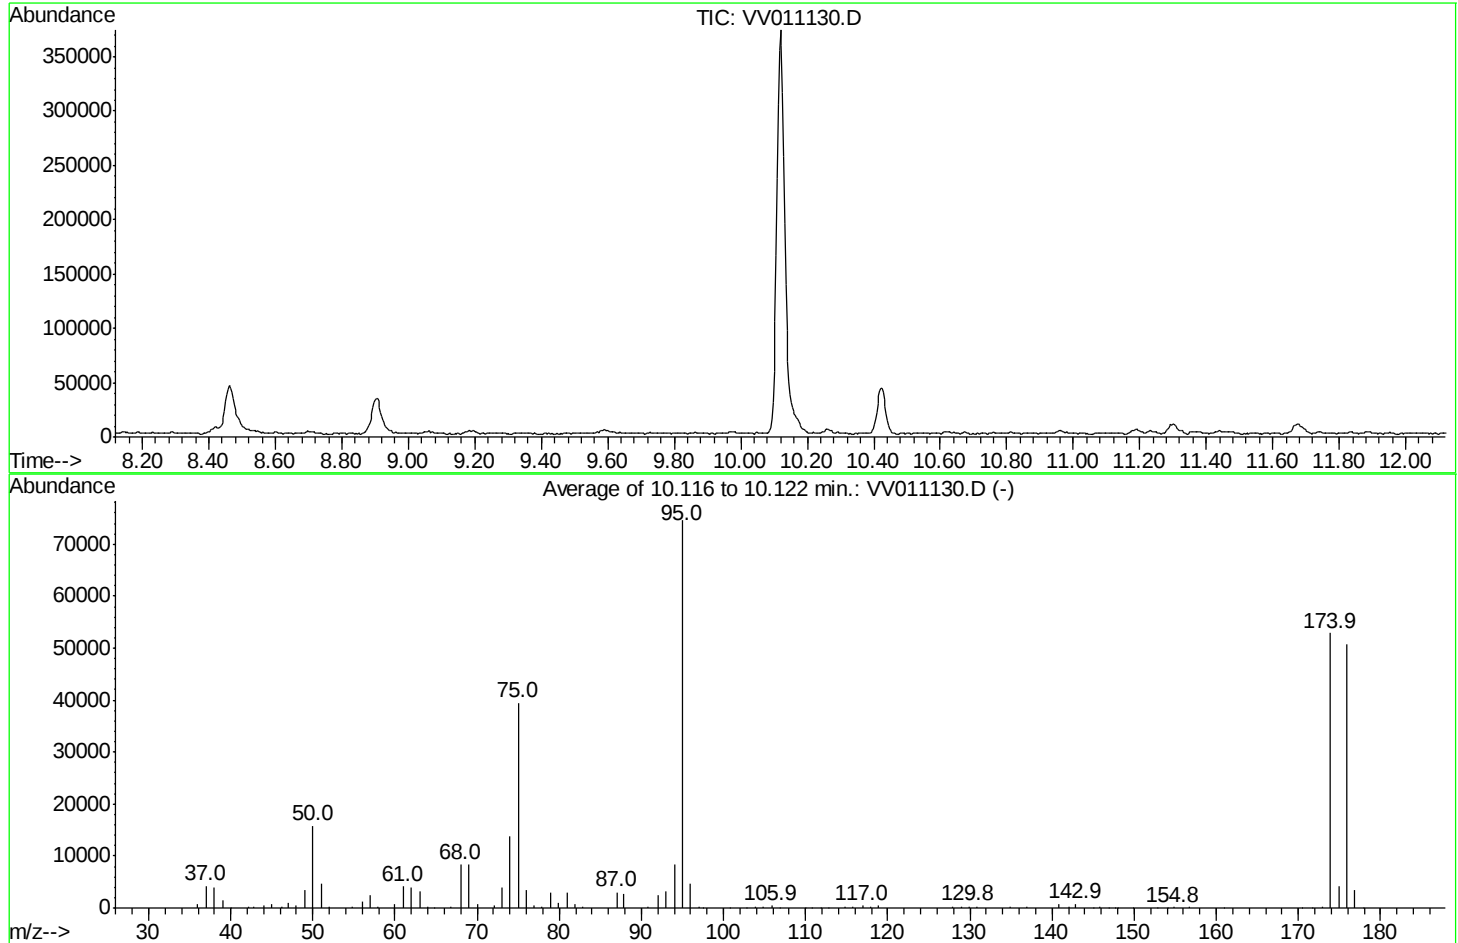

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	15764	PASS
75	95	30	80	52.9	39485	PASS
95	95	100	100	100.0	74586	PASS
96	95	5	9	6.3	4706	PASS
173	174	0.00	2	0.6	310	PASS
174	95	50	120	70.9	52909	PASS
175	174	5	9	7.8	4149	PASS
176	174	95	101	95.7	50637	PASS
177	176	5	9	7.0	3532	PASS

m/z	Abundance
37.00	111.0
37.70	132.0
39.10	174.0
39.90	276.0
40.90	243.0
41.80	149.0
43.00	201.0
43.90	757.0
44.90	121.0
52.50	104.0
53.90	118.0
54.80	123.0
60.10	109.0
69.00	145.0
70.90	125.0
118.90	197.0
168.90	199.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
36.00	800.0
37.00	4400.0
38.00	3865.0
39.00	1707.0
40.00	314.0
41.00	198.0
41.60	121.0
42.10	157.0
43.10	188.0
44.00	1210.0
45.00	867.0
46.20	148.0
47.00	1087.0
47.90	530.0
49.00	3513.0
50.00	15493.0
51.00	4866.0
51.90	319.0
54.90	307.0
56.00	1245.0
57.00	2556.0
57.90	212.0
60.00	894.0
61.00	4040.0
62.00	3967.0
63.00	3008.0
63.90	280.0
66.80	273.0
68.00	8075.0
69.00	8479.0
70.00	828.0
72.00	473.0
73.00	4077.0
74.00	13933.0
75.00	38424.0
76.00	3364.0
76.90	591.0
77.90	279.0
78.90	2848.0
79.90	828.0
80.90	3205.0
81.80	571.0
82.90	166.0
87.00	3000.0
87.90	2642.0
90.80	327.0
92.00	2409.0
92.90	3127.0
94.00	8173.0
95.00	72912.0
96.00	4669.0
97.00	221.0
97.50	111.0
102.80	108.0
104.00	332.0
104.90	178.0
105.90	340.0
106.90	125.0
109.90	125.0
110.70	109.0
114.80	124.0
115.80	266.0
117.00	456.0
117.90	412.0
119.00	604.0
127.80	341.0
128.90	174.0
129.80	327.0
130.80	131.0
134.90	166.0
136.80	179.0
140.90	733.0
142.00	139.0
142.90	868.0
145.80	151.0
146.90	135.0
147.70	139.0
149.80	121.0
154.00	113.0
154.80	134.0
156.70	122.0
161.10	103.0
169.00	149.0
170.50	114.0
173.00	930.0
173.90	50744.0
175.00	4023.0
175.90	48568.0
176.90	3458.0
177.90	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
35.90	824.0
37.00	4573.0
38.00	3998.0
39.00	1813.0
39.90	358.0
41.00	210.0
41.70	128.0
42.10	177.0
42.80	202.0
44.00	1265.0
45.00	902.0
46.20	135.0
46.90	1088.0
47.90	619.0
49.00	3426.0
50.00	16316.0
51.00	4777.0
51.90	344.0
54.90	339.0
56.00	1364.0
57.00	2689.0
57.90	183.0
60.00	887.0
61.00	4336.0
62.00	4058.0
63.00	3289.0
63.90	383.0
66.80	254.0
68.00	8562.0
69.00	8663.0
70.00	769.0
72.00	552.0
73.00	4136.0
74.00	14321.0
75.00	40856.0
76.00	3485.0
76.90	586.0
77.90	307.0
78.90	2944.0
79.90	926.0
80.90	3091.0
81.90	712.0
82.90	165.0
87.00	3163.0
87.90	2762.0
90.90	342.0
92.00	2380.0
92.90	3263.0
94.00	8551.0
95.00	77104.0
96.00	4823.0
96.90	194.0
97.60	108.0
102.70	105.0
103.90	377.0
104.80	193.0
105.90	399.0
106.90	140.0
109.90	133.0
111.80	129.0
114.90	163.0
115.80	314.0
117.00	473.0
117.90	363.0
118.90	607.0
127.80	353.0
128.90	173.0
129.90	379.0
130.90	147.0
134.80	186.0
136.90	175.0
140.90	778.0
142.10	185.0
142.90	878.0
145.00	110.0
145.80	146.0
147.00	133.0
147.80	147.0
149.80	117.0
154.80	166.0
156.80	138.0
160.90	122.0
169.00	193.0
170.50	104.0
171.60	130.0
173.90	54696.0
175.00	4263.0
175.90	52288.0
176.90	3686.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
35.90	832.0
37.00	4307.0
38.00	3851.0
39.10	1728.0
39.90	413.0
40.90	240.0
42.10	166.0
42.80	274.0
44.00	1173.0
45.00	859.0
46.20	122.0
46.90	916.0
47.90	615.0
49.00	3130.0
50.00	15483.0
51.00	4545.0
51.90	317.0
54.90	321.0
56.00	1421.0
57.00	2492.0
57.90	150.0
59.90	853.0
61.00	4167.0
62.00	3771.0
63.00	3290.0
63.90	388.0
64.70	121.0
68.00	8236.0
69.00	8217.0
70.00	713.0
72.10	575.0
73.00	3719.0
74.00	13468.0
75.00	39176.0
76.00	3338.0
76.90	580.0
77.90	300.0
78.90	2844.0
80.00	876.0
80.90	2767.0
82.00	827.0
82.90	143.0
87.00	2928.0
87.90	2631.0
90.90	370.0
92.00	2278.0
92.90	3161.0
94.00	8535.0
95.00	73744.0
96.00	4627.0
96.90	166.0
100.80	109.0
102.70	126.0
103.90	382.0
104.80	199.0
105.90	426.0
106.90	121.0
109.90	129.0
111.80	148.0
112.80	101.0
114.90	171.0
115.80	332.0
116.90	441.0
117.90	316.0
118.90	570.0
127.90	325.0
128.90	155.0
129.90	386.0
130.90	152.0
134.80	203.0
136.90	163.0
140.90	788.0
142.10	184.0
142.90	750.0
145.00	139.0
145.80	127.0
147.00	113.0
148.00	158.0
149.80	109.0
152.90	119.0
154.90	170.0
156.80	145.0
160.90	117.0
169.00	223.0
170.50	108.0
171.70	166.0
173.90	53288.0
174.90	4162.0
175.90	51056.0
176.90	3454.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66