
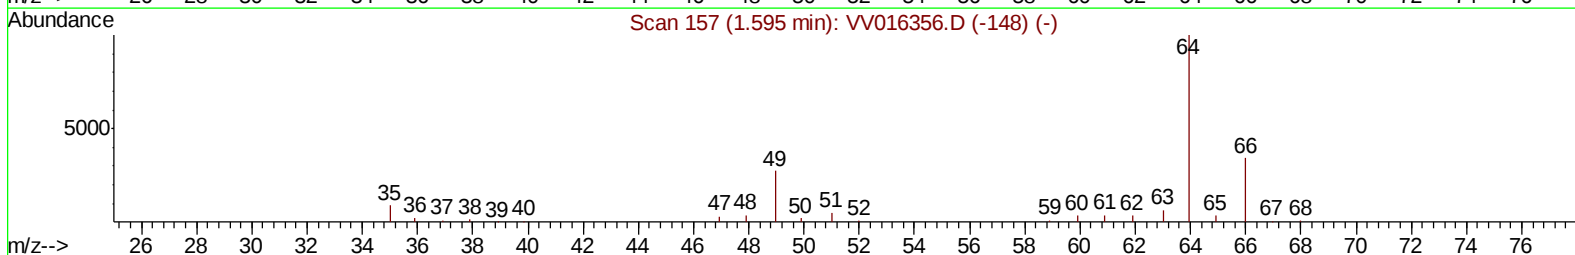
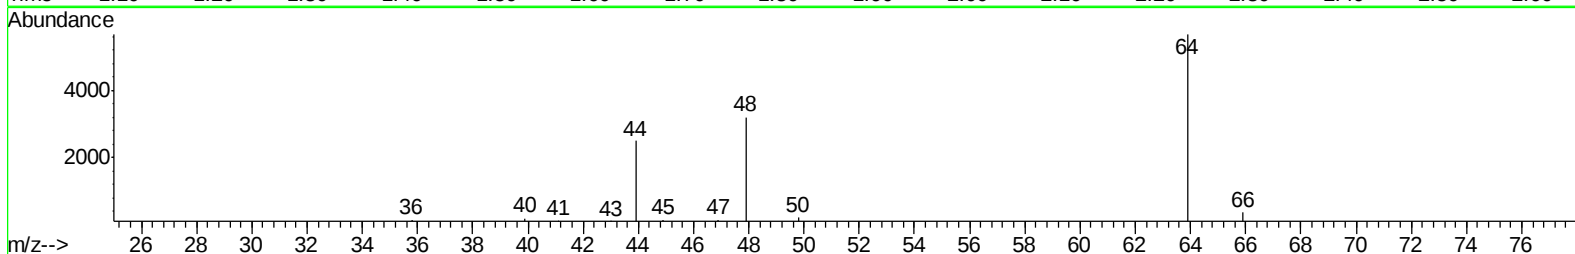


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV053020\
Data File : VV016363.D
Acq On : 30 May 2020 16:37
Operator : SY/MD
Sample : L2662-15
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Jun 01 05:12:21 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 01 05:08:08 2020
Response via : Initial Calibration

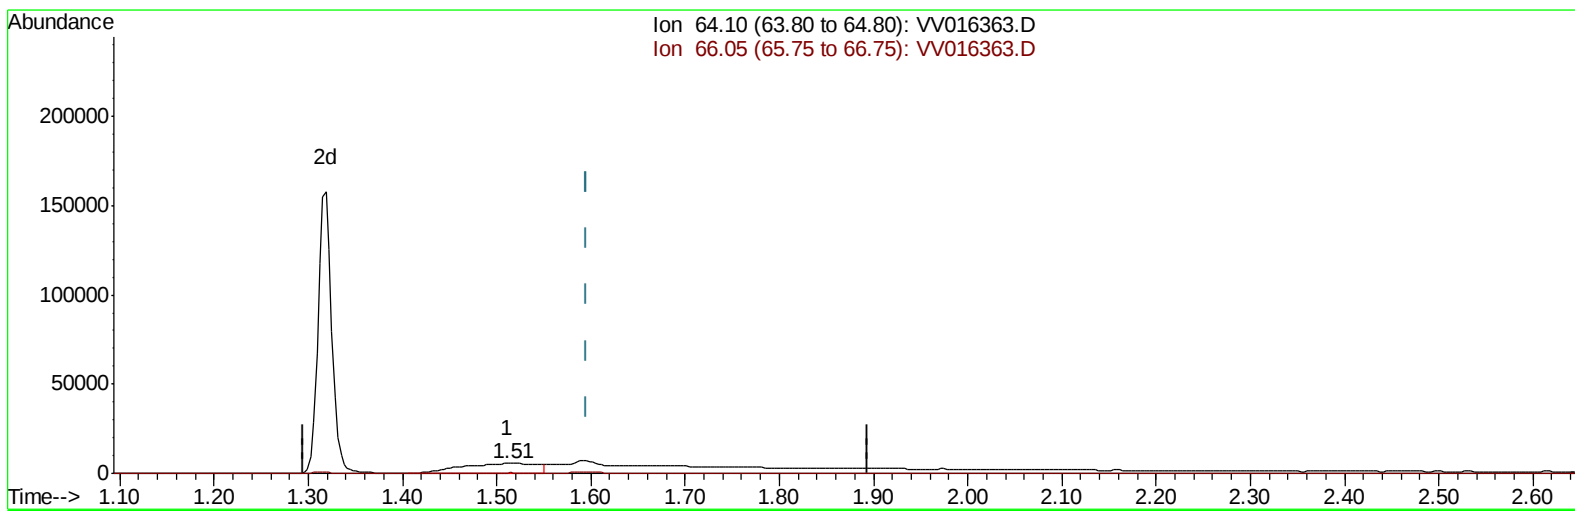

TIC: VV016363.D

(8) Chloroethane (T)

1.512min (-0.084) 7.05ug/L

response 30122

Ion	Exp%	Act%
64.10	100	100
66.05	33.50	6.49#
0.00	0.00	0.00
0.00	0.00	0.00