
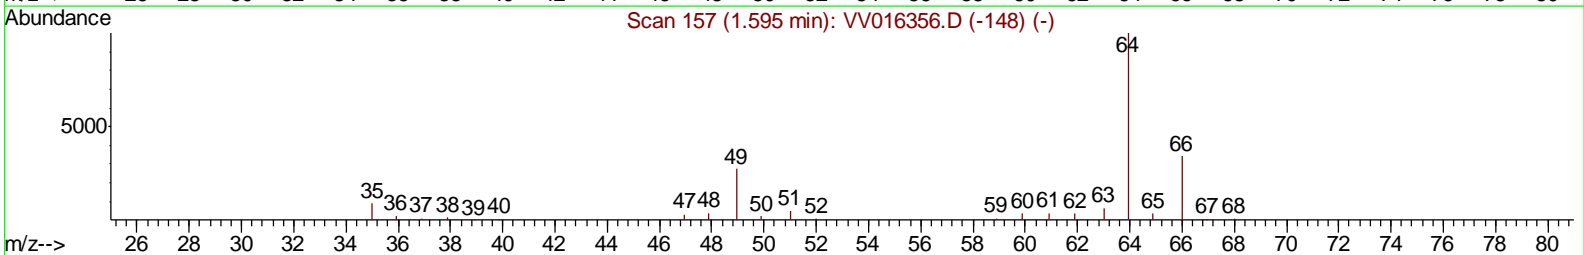
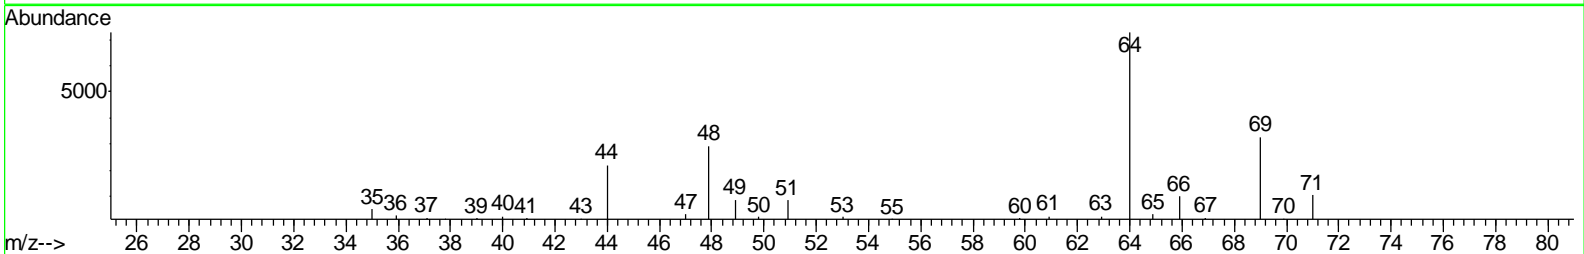


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV053020\  
 Data File : VV016363.D  
 Acq On : 30 May 2020 16:37  
 Operator : SY/MD  
 Sample : L2662-15  
 Misc : 25.0mL/MSVOA V/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Quant Time: Jun 01 05:12:21 2020  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVTR053020WMA.M  
 Quant Title : TRACE VOA SOM01.0  
 QLast Update : Mon Jun 01 05:08:08 2020  
 Response via : Initial Calibration

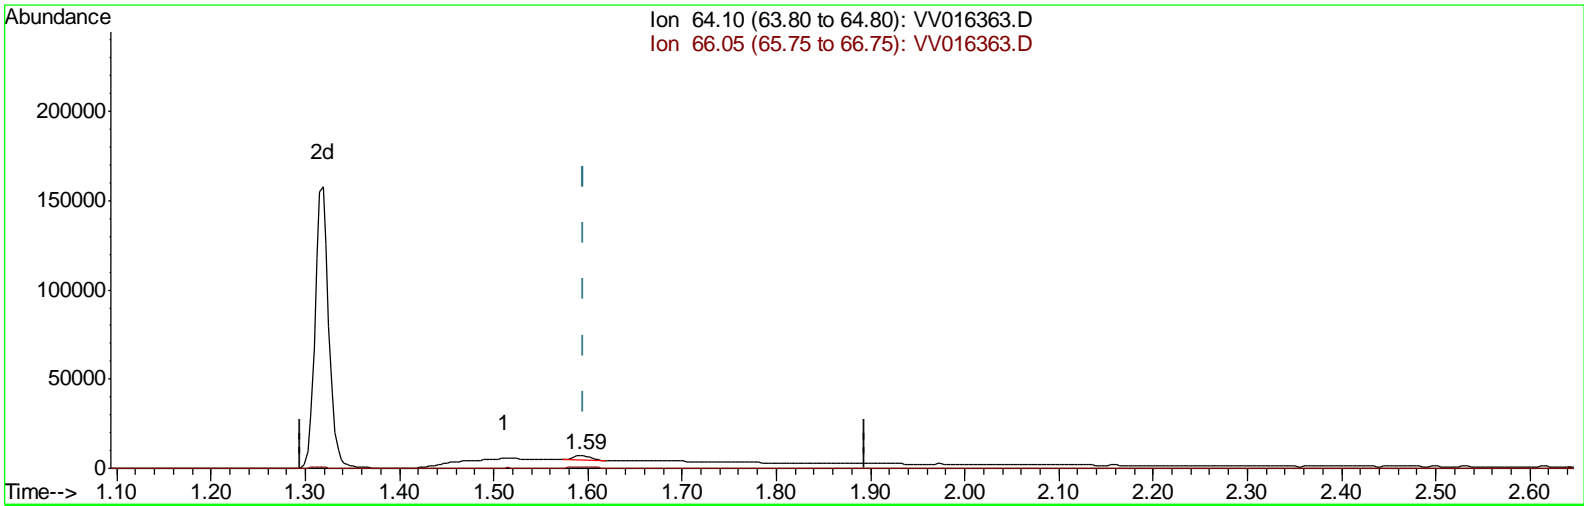

TIC: VV016363.D

(8) Chloroethane (T)

1.592min (-0.003) 0.90ug/L m

response 3866

| Ion   | Exp%  | Act%   |
|-------|-------|--------|
| 64.10 | 100   | 100    |
| 66.05 | 33.50 | 13.61# |
| 0.00  | 0.00  | 0.00   |
| 0.00  | 0.00  | 0.00   |