

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053023\
 Data File : VV031273.D
 Acq On : 30 May 2023 17:36
 Operator : SY/MD
 Sample : 02962-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C11G8

Quant Time: May 31 05:30:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR053023WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 31 05:14:27 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	124968	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	131226	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	56439	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	47809	4.618	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.400%
7) Chloroethane-d5	1.535	69	51453	4.662	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.200%
11) 1,1-Dichloroethene-d2	2.063	65	24289	4.495	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	89.800%
20) 2-Butanone-d5	3.815	46	163610	45.751	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.500%
24) Chloroform-d	4.259	84	116608	4.691	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.800%
26) 1,2-Dichloroethane-d4	4.953	65	64235	4.834	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.600%
32) Benzene-d6	4.969	84	206924	4.360	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.200%
36) 1,2-Dichloropropane-d6	5.998	67	79172	4.727	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.600%
41) Toluene-d8	7.252	98	165059	3.906	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.200%
43) trans-1,3-Dichloroprop...	7.564	79	21911	4.002	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.000%
46) 2-Hexanone-d5	8.034	63	105602	40.842	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.680%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	53495	4.165	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.400%
66) 1,2-Dichlorobenzene-d4	11.567	152	61635	5.255	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.200%
Target Compounds					Qvalue	
13) Acetone	2.140	43	8023	2.731	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053023\
Data File : VV031273.D
Acq On : 30 May 2023 17:36
Operator : SY/MD
Sample : 02962-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C11G8

Quant Time: May 31 05:30:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR053023WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 31 05:14:27 2023
Response via : Initial Calibration

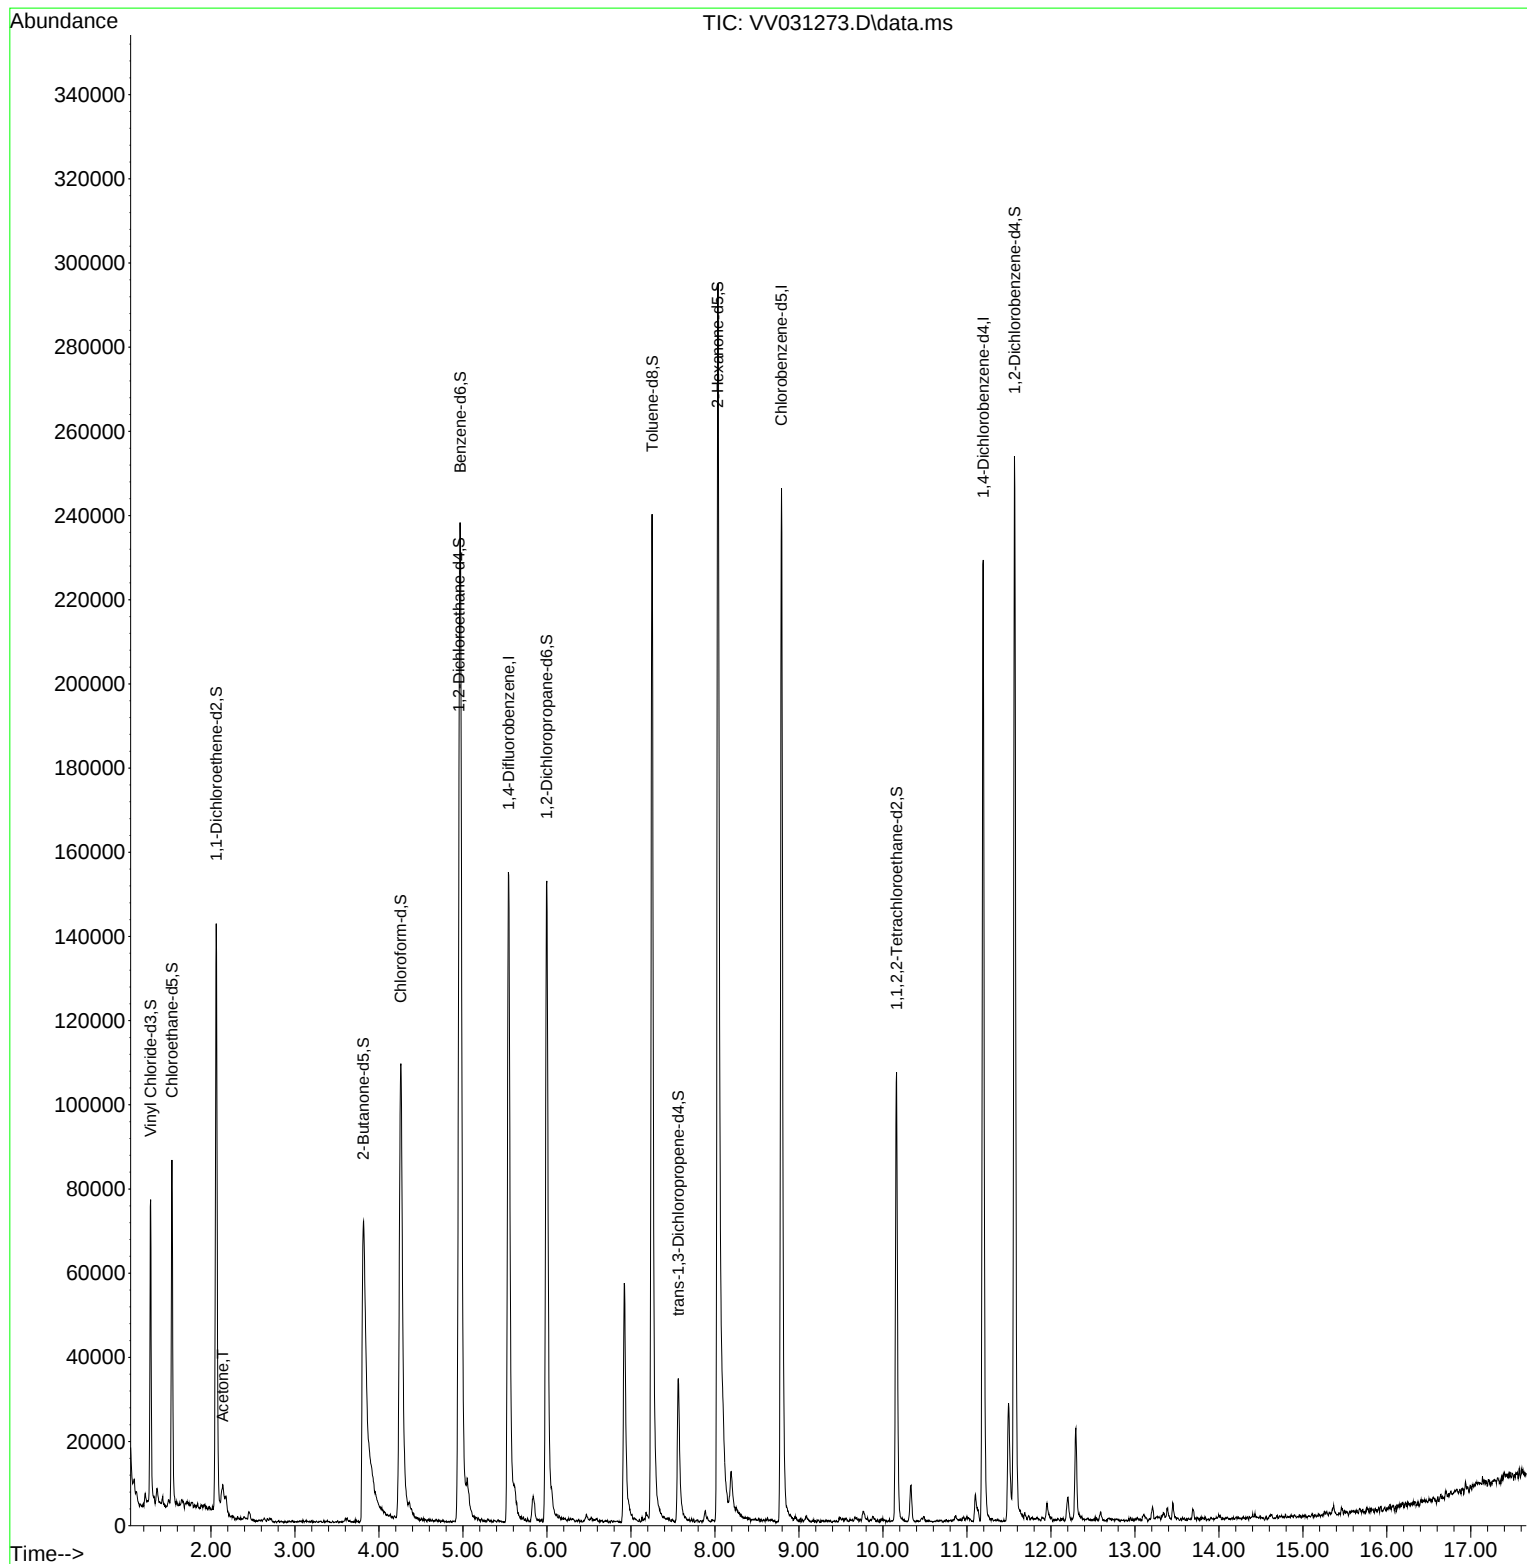

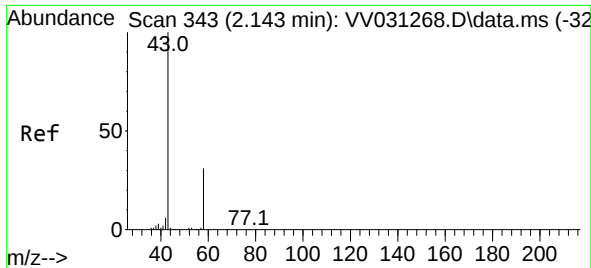

#13

Acetone

Concen: 2.731 ug/L

RT: 2.140 min Scan# 34

Delta R.T. -0.003 min

Lab File: VV031273.D


Acq: 30 May 2023 17:36

Instrument :

MSVOA_V

ClientSampleId :

C11G8

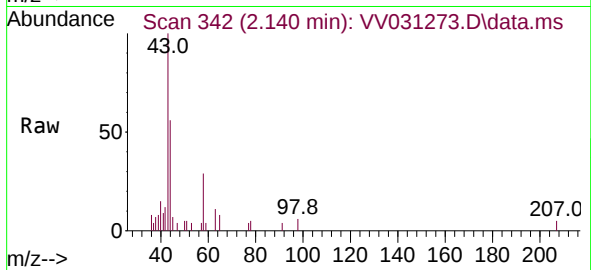

Tgt Ion: 43 Resp: 8023

Ion Ratio Lower Upper

43 100

58 33.6 0.0 64.0

