

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053023\
 Data File : VV031278.D
 Acq On : 30 May 2023 19:40
 Operator : SY/MD
 Sample : 02963-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0P05

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR053023WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031278.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	21	25	35	rVB	12000	14495	1.81%	0.255%
2	1.282	67	75	92	rVB	76548	86635	10.85%	1.521%
3	1.536	147	154	169	rVB	87255	100865	12.63%	1.771%
4	2.063	309	318	333	rVV	142349	206183	25.81%	3.620%
5	2.134	333	340	348	rVV6	5076	10001	1.25%	0.176%
6	2.191	351	358	369	rVB2	7805	13647	1.71%	0.240%
7	3.815	851	863	902	rBV2	80453	311837	39.04%	5.475%
8	4.259	985	1001	1024	rBV	111764	297403	37.23%	5.222%
9	4.966	1204	1221	1244	rBV3	247316	646822	80.98%	11.357%
10	5.056	1245	1249	1270	rVB4	11764	29104	3.64%	0.511%
11	5.542	1387	1400	1417	rBV2	135295	286052	35.81%	5.023%
12	5.844	1481	1494	1512	rBV3	51432	111130	13.91%	1.951%
13	5.998	1528	1542	1559	rBV2	158615	341288	42.73%	5.993%
14	6.921	1818	1829	1856	rBV2	56783	120030	15.03%	2.108%
15	7.252	1920	1932	1945	rBV	247725	457117	57.23%	8.026%
16	7.323	1945	1954	1980	rVB	185201	350311	43.86%	6.151%
17	7.564	2019	2029	2055	rBV	38180	75496	9.45%	1.326%
18	8.037	2162	2176	2215	rBV	356751	798747	100.00%	14.025%
19	8.793	2399	2411	2439	rBV	219613	386209	48.35%	6.781%
20	9.085	2493	2502	2513	rBV3	7349	12704	1.59%	0.223%
21	10.162	2824	2837	2856	rBV	131243	213860	26.77%	3.755%
22	10.333	2881	2890	2903	rVB2	13413	22136	2.77%	0.389%
23	11.194	3135	3158	3181	rBV	206394	349191	43.72%	6.131%
24	11.500	3242	3253	3263	rBV3	10392	19342	2.42%	0.340%
25	11.567	3263	3274	3300	rVB	256388	422975	52.95%	7.427%
26	12.207	3463	3473	3483	rVB2	6962	11604	1.45%	0.204%




Sum of corrected areas: 5695184

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053023\
Data File : VV031278.D
Acq On : 30 May 2023 19:40
Operator : SY/MD
Sample : 02963-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0P05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR053023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

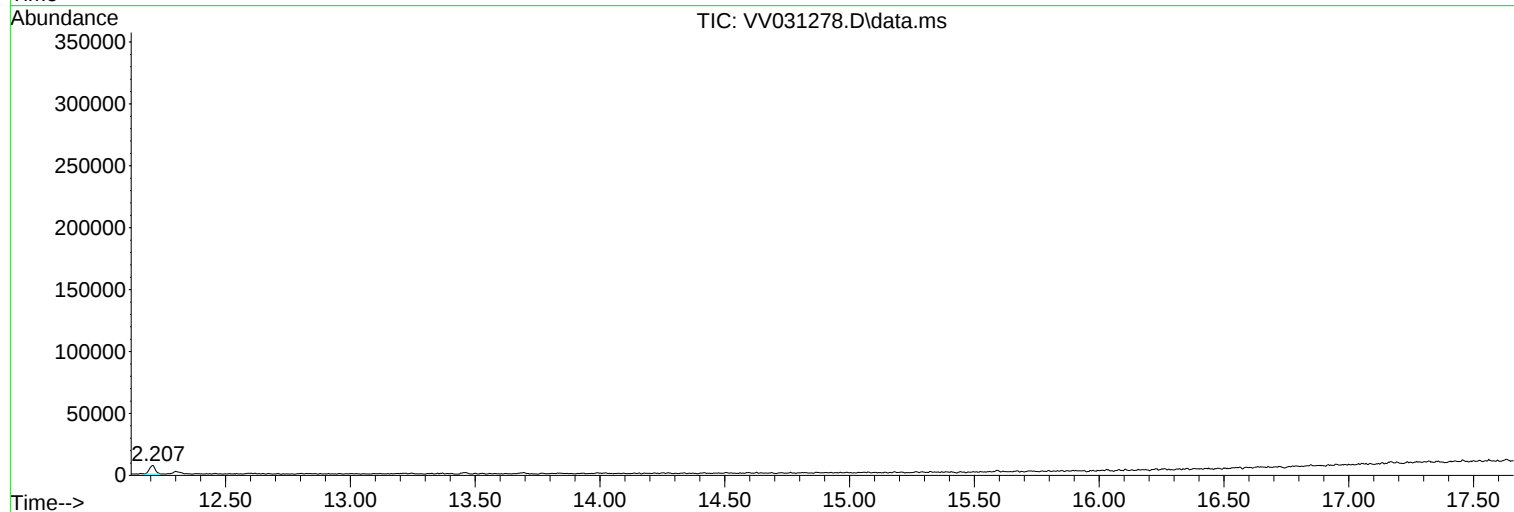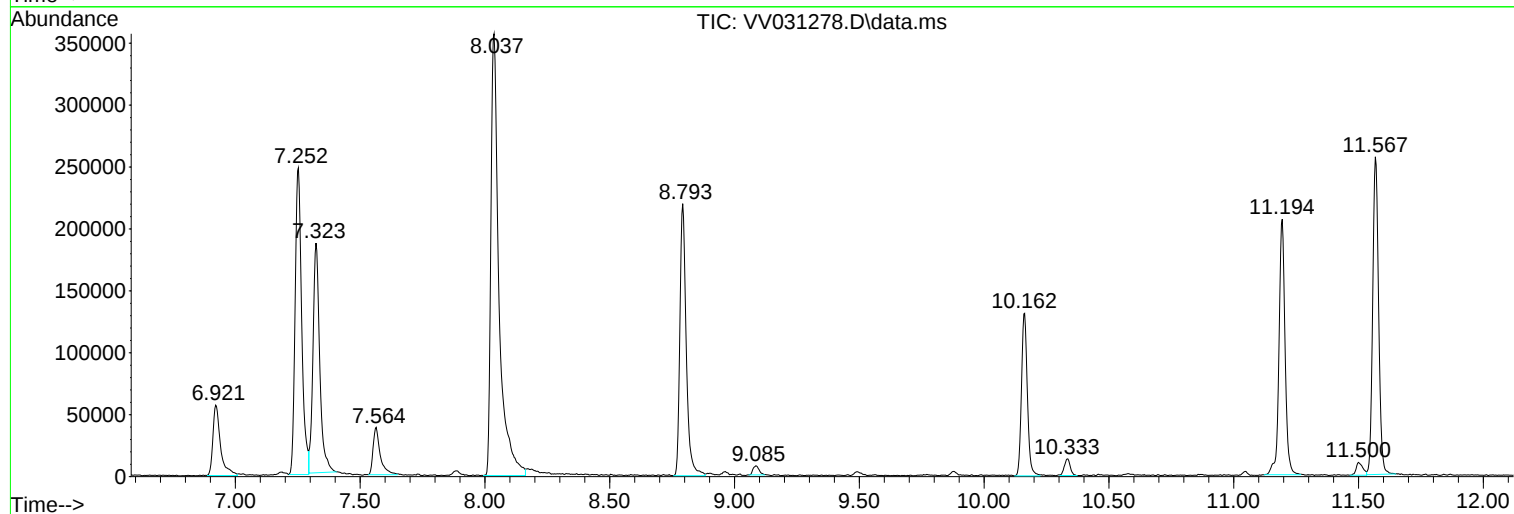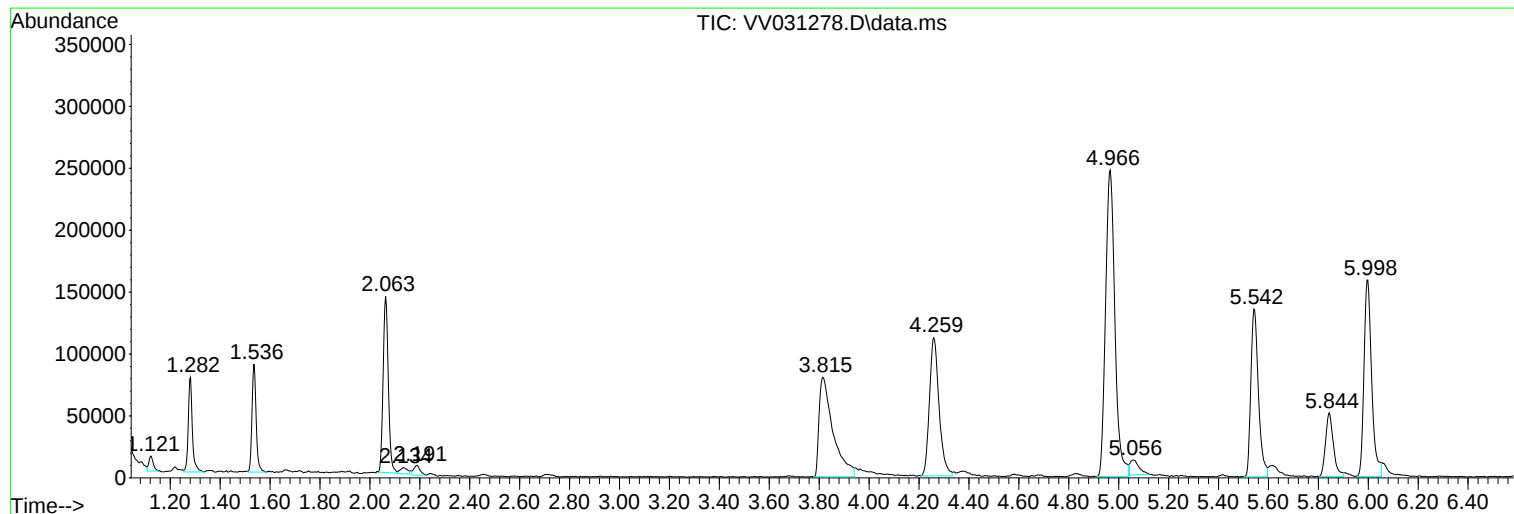

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053023\
Data File : VV031278.D
Acq On : 30 May 2023 19:40
Operator : SY/MD
Sample : 02963-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0P05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR053023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053023\
Data File : VV031278.D
Acq On : 30 May 2023 19:40
Operator : SY/MD
Sample : 02963-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0P05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR053023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc