


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053023\
Data File : VV031265.D
Acq On : 30 May 2023 13:52
Operator : SY/MD
Sample : BFB267
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB267

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR053023WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed May 31 05:14:27 2023

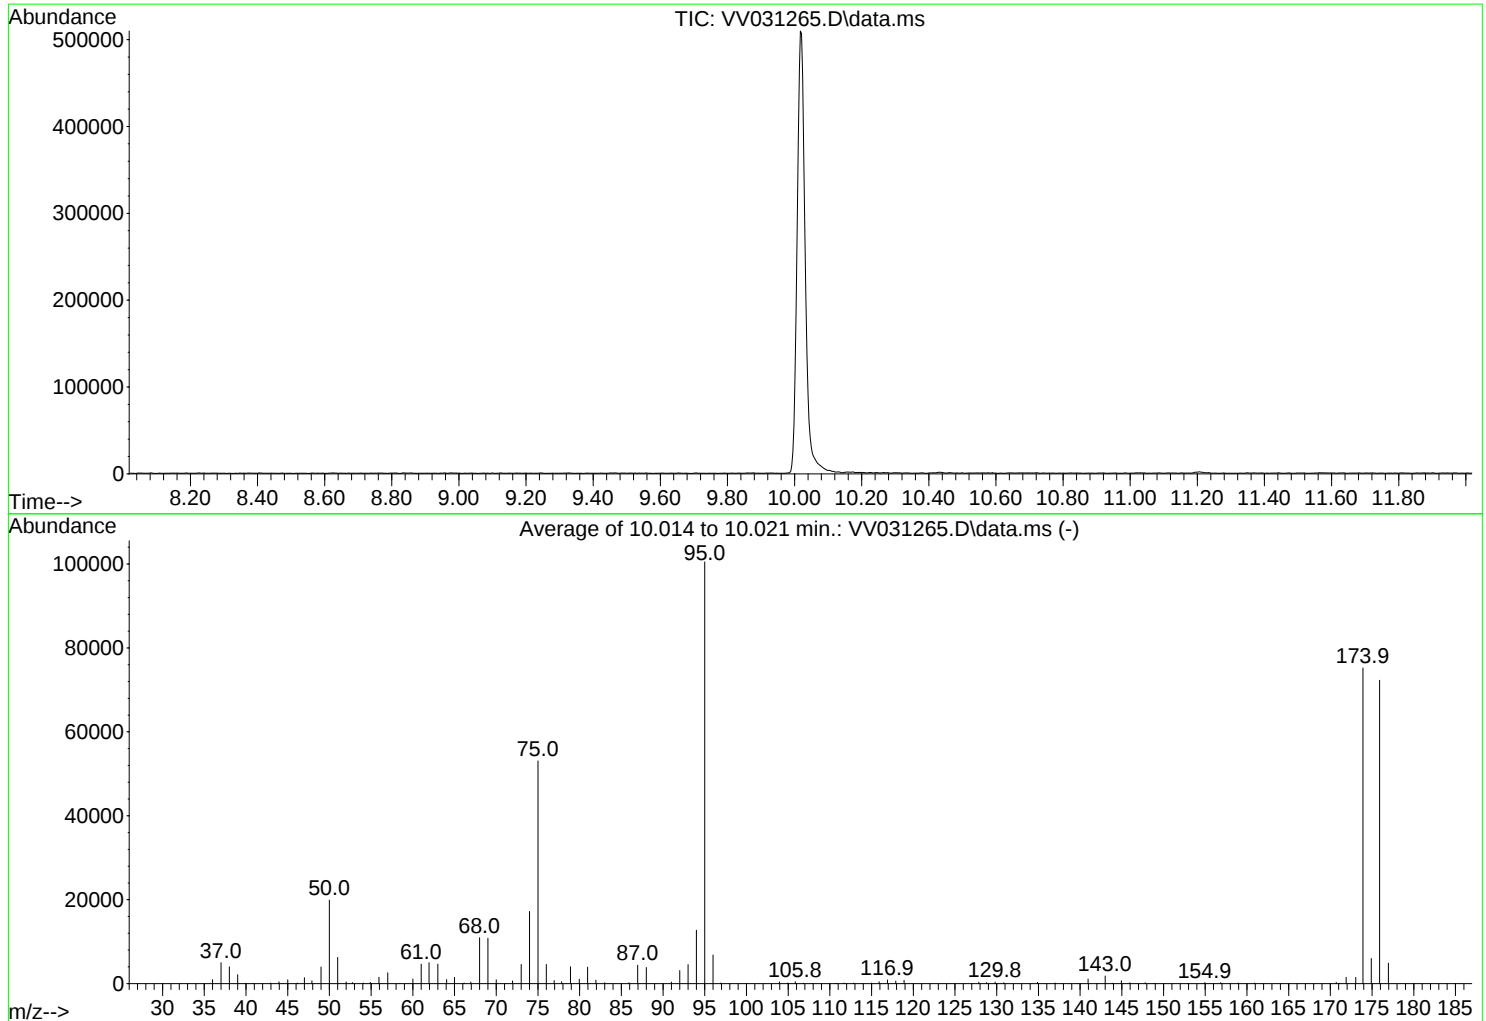

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	19888	PASS
75	95	30	80	52.8	53072	PASS
95	95	100	100	100.0	100517	PASS
96	95	5	9	6.8	6821	PASS
173	174	0.00	2	2.0	1499	PASS
174	95	50	120	74.9	75251	PASS
175	174	5	9	8.0	5992	PASS
176	174	95	105	96.1	72283	PASS
177	176	5	10	6.7	4873	PASS

m/z	Abundance
39.90	417.0
44.00	363.0

Instrument :
MSVOA_V
ClientSampleId :
BFB267

m/z	Abundance
36.00	918.0
37.00	4762.0
38.00	3826.0
39.00	1943.0
39.90	507.0
40.90	113.0
43.00	141.0
43.90	784.0
45.00	834.0
46.10	219.0
47.00	1286.0
47.90	767.0
49.00	3647.0
50.00	19224.0
51.00	6182.0
52.00	318.0
52.80	266.0
54.10	122.0
54.90	289.0
56.00	1388.0
57.00	2520.0
58.40	157.0
60.00	968.0
61.00	4553.0
61.90	4907.0
63.00	4409.0
64.10	848.0
65.00	1302.0
66.20	104.0
67.00	435.0
68.00	10545.0
69.00	10038.0
70.00	849.0
72.00	686.0
73.00	4534.0
74.00	16624.0
75.00	50432.0
76.00	4487.0
77.00	764.0
77.90	420.0
78.90	3838.0
79.90	984.0
80.90	3728.0
81.90	802.0
83.00	211.0
86.00	181.0
86.90	4213.0
88.00	3592.0
91.00	432.0
92.00	3068.0
93.00	4497.0
94.00	12214.0
95.00	95240.0
96.00	6518.0
96.90	167.0
103.90	368.0
105.00	175.0
105.80	464.0
106.90	114.0
110.70	105.0
111.70	138.0
112.80	122.0
115.10	177.0
115.90	495.0
116.90	820.0
117.90	602.0
118.90	777.0
127.80	296.0
128.90	270.0
129.80	371.0
130.80	210.0
134.90	290.0
137.00	168.0
141.00	1039.0
143.00	1844.0
143.80	122.0
145.00	616.0
146.00	162.0
147.80	182.0
154.90	273.0
156.90	234.0
158.90	167.0
160.90	158.0
170.60	272.0
171.10	216.0
171.90	1359.0
173.00	1441.0
173.90	68976.0
174.90	5622.0
175.90	67008.0
176.90	4625.0

Instrument :
MSVOA_V
ClientSampleId :
BFB267

m/z	Abundance
36.00	994.0
37.00	5273.0
38.00	4101.0
39.00	2219.0
40.00	469.0
42.90	149.0
44.00	792.0
45.00	946.0
46.20	220.0
47.00	1464.0
47.90	706.0
49.00	4034.0
50.00	20528.0
51.00	6497.0
52.00	447.0
52.80	276.0
54.10	143.0
54.90	326.0
56.00	1540.0
57.00	2649.0
58.50	109.0
60.00	1128.0
61.00	4749.0
62.00	5159.0
63.00	4777.0
64.10	997.0
65.00	1528.0
66.20	157.0
66.90	397.0
68.00	11328.0
69.00	11176.0
70.00	969.0
72.00	647.0
73.00	4741.0
74.00	17720.0
75.00	54592.0
76.00	4757.0
76.90	729.0
77.80	440.0
78.90	4108.0
80.00	1114.0
80.90	4044.0
81.90	863.0
83.00	224.0
85.90	224.0
86.90	4513.0
88.00	3895.0
91.00	380.0
92.00	3193.0
93.00	4649.0
94.00	13392.0
95.00	103752.0
96.00	7093.0
96.90	162.0
104.00	418.0
104.90	151.0
105.80	478.0
106.90	118.0
110.90	108.0
111.70	142.0
112.80	151.0
115.00	145.0
115.90	502.0
116.90	877.0
117.90	630.0
118.90	837.0
127.90	356.0
128.80	237.0
129.80	416.0
130.80	235.0
134.90	351.0
137.00	166.0
140.90	1122.0
143.00	1901.0
143.80	106.0
144.90	704.0
145.90	226.0
147.80	210.0
148.90	106.0
152.90	127.0
155.00	270.0
156.80	271.0
159.00	159.0
160.90	158.0
170.70	289.0
171.90	1603.0
173.00	1547.0
173.90	77624.0
174.90	6144.0
175.90	74576.0
176.90	5011.0

Instrument :
MSVOA_V
ClientSampleId :
BFB267

m/z	Abundance
36.00	932.0
37.00	4975.0
38.00	4111.0
39.00	2286.0
40.00	507.0
40.80	120.0
42.90	164.0
44.00	797.0
45.00	931.0
47.00	1441.0
47.90	576.0
49.00	4262.0
50.00	19912.0
51.00	6130.0
52.00	495.0
52.70	227.0
54.10	156.0
54.90	290.0
55.90	1611.0
57.00	2601.0
60.00	1199.0
61.00	4619.0
62.00	4979.0
63.00	4736.0
64.00	1045.0
65.00	1613.0
66.10	158.0
66.90	263.0
68.00	11010.0
69.00	11234.0
70.00	929.0
71.90	607.0
73.00	4460.0
74.00	17280.0
75.00	54192.0
76.00	4504.0
76.90	690.0
77.80	529.0
78.90	4061.0
80.00	1126.0
81.00	4059.0
82.00	849.0
83.00	200.0
85.80	256.0
87.00	4395.0
88.00	4042.0
91.00	352.0
92.00	3105.0
93.00	4523.0
94.00	12586.0
95.00	102560.0
96.00	6853.0
96.90	152.0
103.90	440.0
104.90	107.0
105.90	451.0
106.80	104.0
107.90	102.0
110.60	120.0
110.90	134.0
111.70	133.0
112.90	180.0
114.90	155.0
115.90	434.0
116.90	890.0
117.90	588.0
118.90	755.0
127.90	409.0
128.70	248.0
129.80	377.0
130.90	193.0
134.90	298.0
137.00	173.0
139.70	123.0
140.90	1151.0
142.10	140.0
143.00	1777.0
143.90	122.0
144.90	736.0
145.90	255.0
147.80	255.0
148.80	133.0
152.90	123.0
155.00	230.0
156.80	219.0
159.00	143.0
160.90	135.0
170.00	118.0
170.80	330.0
171.90	1659.0
173.10	1510.0
173.90	79152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB267

174.90	6211.0
175.90	75264.0
177.00	4984.0

Instrument :
MSVOA_V
ClientSampleId :
BFB267