


Data Path : W:\HPCHEM1\MSVOA V\DATA\VV053118\
 Data File : VV006113.D
 Acq On : 31 May 2018 16:44
 Operator : SY/MD
 Sample : BFB01
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB01

Integration File: rteint.p

Method : W:\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Jun 04 00:26:11 2018

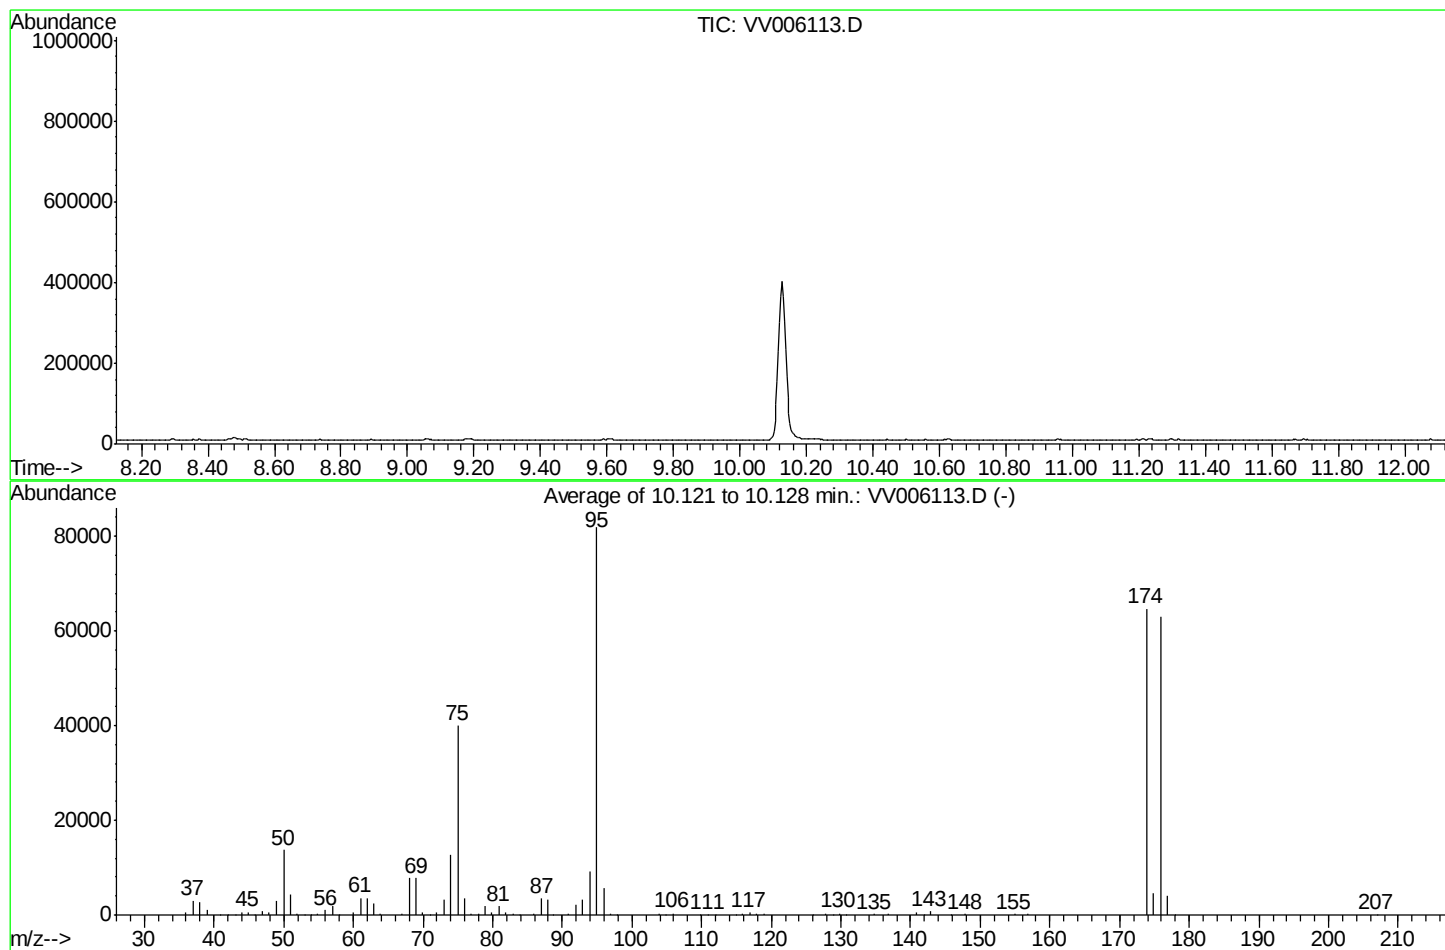

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2855

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	13789	PASS
75	95	30	80	48.8	39938	PASS
95	95	100	100	100.0	81889	PASS
96	95	5	9	6.9	5667	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.1	64757	PASS
175	174	5	9	7.3	4713	PASS
176	174	95	101	97.1	62882	PASS
177	176	5	9	6.4	4051	PASS

m/z	Abundance
38.00	100.0
38.90	443.0
39.90	244.0
41.00	582.0
42.00	481.0
43.00	1087.0
44.00	1474.0
44.90	429.0
45.90	173.0
50.00	109.0
50.90	102.0
52.10	120.0
53.00	193.0
53.90	117.0
54.90	555.0
56.00	287.0
57.00	381.0
58.00	155.0
60.00	303.0
67.10	135.0
69.00	369.0
69.90	157.0
71.00	136.0
73.10	185.0
77.00	169.0
78.80	118.0
80.90	157.0
82.00	123.0
83.80	114.0
85.00	281.0
91.00	146.0
94.90	113.0
95.80	141.0
97.00	156.0
97.90	196.0
125.90	121.0
207.00	238.0

Instrument :
MSVOA_V
ClientSampleId :
BFB01

m/z	Abundance
36.00	590.0
37.00	3002.0
38.00	2698.0
39.00	1454.0
39.90	247.0
40.90	651.0
41.90	490.0
43.00	1123.0
43.90	1951.0
44.90	948.0
46.00	241.0
47.00	679.0
47.90	413.0
49.00	2788.0
50.00	13260.0
51.00	4302.0
51.90	319.0
53.00	241.0
54.00	167.0
54.90	711.0
56.00	1349.0
57.00	2178.0
58.10	184.0
59.90	825.0
61.00	3556.0
62.00	3358.0
63.00	2493.0
63.90	290.0
67.00	313.0
68.00	7399.0
69.00	7633.0
70.00	800.0
70.90	169.0
72.00	448.0
73.00	3189.0
74.00	12270.0
75.00	37480.0
76.00	3343.0
76.90	477.0
77.90	385.0
78.90	1961.0
79.90	577.0
80.90	1993.0
81.90	531.0
82.90	171.0
84.00	167.0
85.00	271.0
86.00	151.0
87.00	3216.0
87.90	2979.0
90.90	296.0
92.00	1950.0
92.90	3036.0
94.00	8647.0
95.00	77008.0
96.00	5668.0
97.00	305.0
97.90	320.0
103.80	305.0
104.90	151.0
105.90	277.0
109.90	126.0
110.90	121.0
111.90	112.0
114.90	142.0
115.90	245.0
116.90	462.0
117.80	290.0
118.90	333.0
126.00	134.0
127.70	199.0
128.90	146.0
129.80	254.0
130.70	129.0
134.90	159.0
136.90	139.0
140.90	658.0
141.80	103.0
142.90	667.0
145.90	112.0
147.90	176.0
155.00	162.0
156.80	133.0
173.90	59496.0
174.90	4382.0
175.90	57440.0
176.90	3816.0
177.90	109.0
206.90	273.0

Instrument :
MSVOA_V
ClientSampleId :
BFB01

m/z	Abundance
36.00	591.0
37.00	3129.0
38.00	2855.0
39.00	1486.0
39.90	241.0
40.90	701.0
41.90	552.0
43.00	1119.0
43.90	2015.0
44.90	1018.0
46.00	207.0
47.00	776.0
47.90	547.0
49.00	2964.0
50.00	14345.0
51.00	4717.0
52.00	350.0
53.00	242.0
54.00	161.0
55.00	706.0
56.00	1398.0
57.00	2327.0
58.10	220.0
59.90	860.0
61.00	3702.0
62.00	3689.0
63.00	2597.0
63.90	292.0
67.00	337.0
68.00	7995.0
69.00	8447.0
70.00	816.0
70.90	167.0
72.00	524.0
73.00	3450.0
74.00	13201.0
75.00	41288.0
76.00	3591.0
77.00	495.0
77.90	411.0
78.90	2093.0
79.90	642.0
80.90	2109.0
81.80	569.0
83.00	197.0
84.00	151.0
85.00	243.0
85.90	165.0
87.00	3591.0
87.90	3389.0
90.90	356.0
91.90	2215.0
92.90	3265.0
94.00	9377.0
95.00	84728.0
96.00	5994.0
97.00	334.0
98.00	300.0
103.80	326.0
104.90	135.0
105.90	343.0
109.80	125.0
110.90	114.0
114.90	144.0
115.90	296.0
116.90	513.0
117.80	315.0
118.90	373.0
126.00	141.0
127.70	223.0
128.90	135.0
129.80	287.0
130.70	133.0
134.80	158.0
136.80	153.0
140.90	697.0
141.80	116.0
142.80	742.0
145.90	121.0
147.90	194.0
155.00	204.0
156.80	157.0
173.90	66608.0
174.90	4914.0
175.90	64744.0
176.90	4161.0
177.90	116.0
206.90	290.0

Instrument :
MSVOA_V
ClientSampleId :
BFB01

m/z	Abundance
36.00	597.0
37.00	3051.0
38.00	2839.0
39.00	1466.0
39.90	227.0
40.90	765.0
41.90	505.0
43.00	1149.0
44.00	2026.0
45.00	1050.0
45.90	183.0
47.00	826.0
47.90	576.0
49.00	2899.0
50.00	14090.0
51.00	4602.0
52.00	317.0
53.00	232.0
54.00	147.0
55.00	735.0
56.00	1346.0
57.00	2365.0
58.10	215.0
59.90	852.0
61.00	3475.0
62.00	3610.0
63.00	2489.0
63.90	259.0
67.10	321.0
68.00	7841.0
69.00	8380.0
70.00	792.0
71.00	160.0
72.00	465.0
73.00	3425.0
74.00	12927.0
75.00	41048.0
76.00	3461.0
77.00	448.0
77.90	412.0
78.90	1966.0
79.90	684.0
80.90	2017.0
81.80	550.0
83.00	208.0
83.90	153.0
85.00	238.0
85.90	160.0
87.00	3655.0
87.90	3389.0
88.70	132.0
90.90	392.0
91.90	2318.0
93.00	3233.0
94.00	9409.0
95.00	84272.0
96.00	5762.0
97.00	323.0
98.00	269.0
103.90	329.0
104.90	119.0
105.90	355.0
110.90	114.0
114.80	135.0
115.90	295.0
116.90	498.0
117.80	284.0
118.90	377.0
126.00	135.0
127.80	231.0
129.00	147.0
129.80	280.0
130.80	130.0
134.80	139.0
136.80	142.0
140.90	684.0
141.90	112.0
142.80	732.0
145.80	126.0
147.90	195.0
154.90	242.0
156.80	150.0
173.90	68168.0
174.90	4845.0
175.90	66464.0
176.90	4176.0
177.90	110.0
206.90	291.0

Instrument :
MSVOA_V
ClientSampleId :
BFB01