

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV053119\
 Data File : VV011189.D
 Acq On : 31 May 2019 21:29
 Operator : SY/MD
 Sample : VIBLK46
 Misc : 5.00G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK46

Quant Time: Jun 01 01:19:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM053019S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 01 00:27:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	302202	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	293765	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	135603	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	81440	19.92	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.68%
7) Chloroethane-d5	1.57	69	69623	22.15	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.60%
10) 1,1-Dichloroethene-d2	2.12	63	132449	15.78	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.12%
20) 2-Butanone-d5	3.94	46	66286	44.35	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.70%
24) Chloroform-d	4.40	84	167080	22.62	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.48%
26) 1,2-Dichloroethane-d4	5.08	65	113783	23.64	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.56%
29) Benzene-d6	5.09	84	359299	22.52	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.08%
33) 1,2-Dichloropropane-d6	6.12	67	117963	23.08	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.32%
37) Toluene-d8	7.36	98	327880	21.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.12%
38) trans-1,3-Dichloropropene-	7.66	79	45331	19.60	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.40%
39) 2-Hexanone-d5	8.13	63	49900	42.95	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.90%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	103681	22.51	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.04%
61) 1,2-Dichlorobenzene-d4	11.67	152	121183	23.88	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.52%


Target Compounds					Ovalue
13) Acetone	2.19	43	5139	2.956 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV053119\
Data File : VV011189.D
Acq On : 31 May 2019 21:29
Operator : SY/MD
Sample : VIBLK46
Misc : 5.00G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK46

Quant Time: Jun 01 01:19:10 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM053019S.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 01 00:27:53 2019
Response via : Initial Calibration

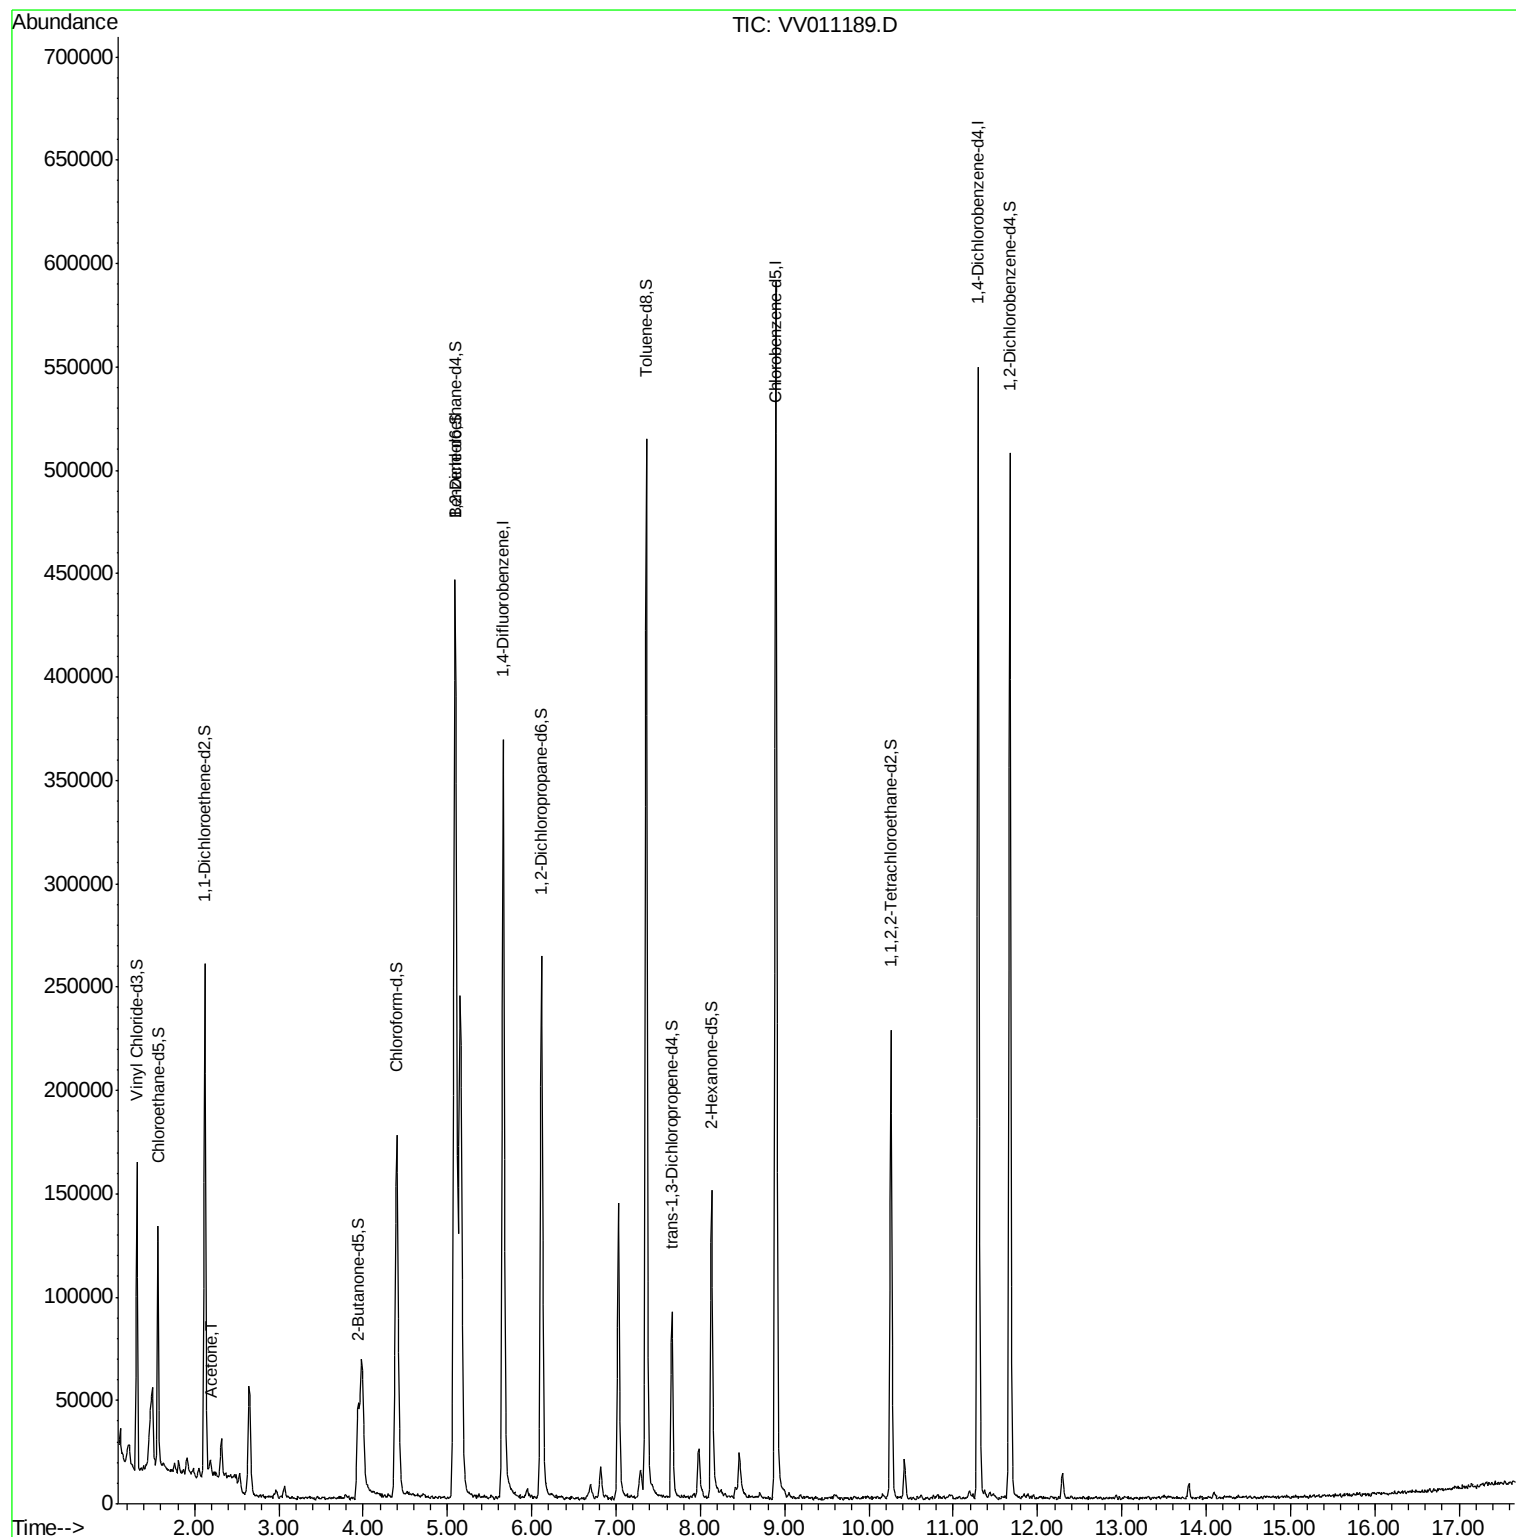

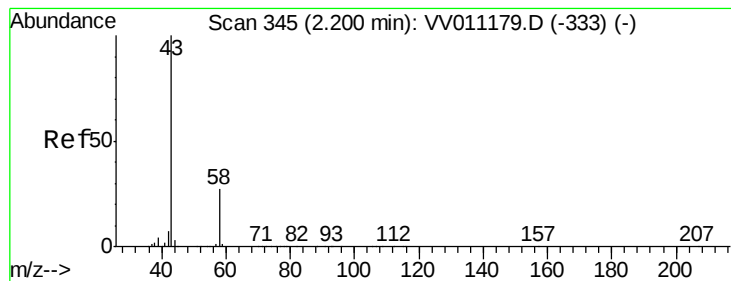

#13
 Acetone
 Concen: 2.956 ug/L
 RT: 2.19 min Scan# 342
 Delta R.T. -0.01 min
 Lab File: VV011189.D
 Acq: 31 May 2019 21:29

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK46

Tot Ion: 43 Resp: 5139
 Ion Ratio Lower Upper
 43 100
 58 29.2 0.0 53.8

