


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV053119\
 Data File : VV011178.D
 Acq On : 31 May 2019 14:49
 Operator : SY/MD
 Sample : BFB67
 Misc : 5.00G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB67

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM053019S.M
 Title : VOC Analysis
 Last Update : Mon Jun 03 05:47:22 2019

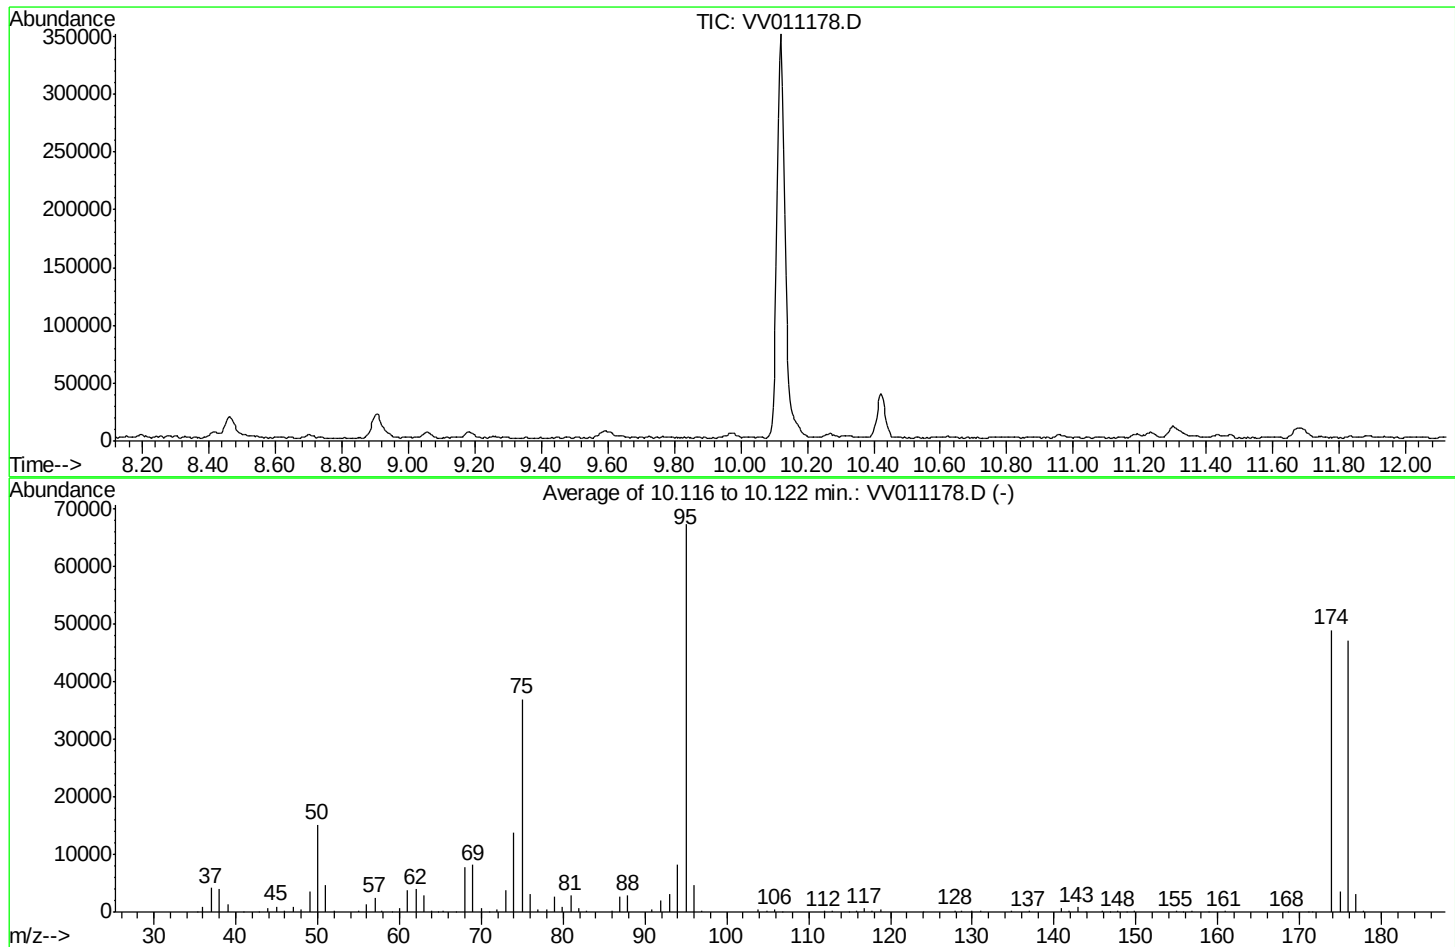

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	15227	PASS
75	95	30	80	55.0	37034	PASS
95	95	100	100	100.0	67376	PASS
96	95	5	9	7.0	4705	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.8	49053	PASS
175	174	5	9	7.4	3629	PASS
176	174	95	101	96.0	47074	PASS
177	176	5	9	6.8	3190	PASS

m/z	Abundance
39.00	135.0
39.90	394.0
41.00	133.0
41.90	171.0
42.80	157.0
44.00	580.0
45.20	115.0
48.10	103.0
52.30	104.0
66.90	119.0
68.90	140.0
84.20	120.0
119.00	110.0
168.90	194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
35.30	140.0
36.00	832.0
37.00	4211.0
38.00	3906.0
39.00	1463.0
40.10	271.0
41.00	171.0
42.10	120.0
43.00	152.0
43.90	1226.0
45.00	1093.0
45.90	119.0
47.00	980.0
48.00	577.0
49.00	3432.0
50.00	14773.0
51.00	4599.0
51.90	290.0
54.90	243.0
56.00	1256.0
57.00	2495.0
57.80	147.0
59.90	731.0
61.00	3698.0
62.00	3988.0
63.00	2780.0
63.90	336.0
65.40	108.0
66.90	233.0
68.00	7842.0
69.00	7940.0
69.90	621.0
70.90	116.0
72.00	497.0
73.00	3636.0
74.00	13566.0
75.00	35656.0
76.00	3114.0
76.90	531.0
77.90	392.0
78.90	2586.0
80.00	840.0
80.90	2746.0
81.90	603.0
82.80	108.0
86.00	169.0
86.90	2597.0
87.90	2614.0
90.80	434.0
91.90	1974.0
93.00	3234.0
94.00	7609.0
95.00	65360.0
96.00	4534.0
96.90	145.0
103.80	358.0
104.90	145.0
105.80	457.0
106.90	103.0
111.90	128.0
112.90	164.0
114.90	118.0
115.80	306.0
116.80	533.0
117.80	293.0
118.90	527.0
127.90	346.0
128.80	167.0
129.90	247.0
131.00	151.0
134.90	208.0
136.90	186.0
140.90	721.0
141.70	203.0
142.90	890.0
145.90	204.0
146.80	107.0
147.80	160.0
149.80	175.0
154.90	164.0
155.80	106.0
156.80	151.0
158.90	111.0
160.90	107.0
168.50	119.0
169.00	195.0
171.10	103.0
171.60	173.0
173.90	45960.0
174.90	3407.0
175.90	44192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

176.902900.0

177.80114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
36.00	735.0
37.00	4043.0
38.00	3961.0
39.00	1516.0
39.90	259.0
40.20	247.0
41.00	180.0
42.00	141.0
42.80	184.0
43.90	1301.0
45.00	952.0
45.90	151.0
47.00	902.0
48.00	563.0
49.00	3503.0
50.00	15133.0
51.00	4540.0
52.10	236.0
55.00	281.0
56.00	1505.0
57.00	2497.0
57.90	160.0
60.00	704.0
61.00	3915.0
62.00	3722.0
63.00	2865.0
64.00	307.0
65.40	132.0
67.00	162.0
68.00	7605.0
69.00	8404.0
70.00	635.0
71.90	566.0
73.00	3643.0
74.00	13628.0
75.00	37280.0
76.00	3046.0
77.00	558.0
78.00	390.0
78.90	2484.0
79.90	770.0
80.90	2874.0
81.90	685.0
82.90	136.0
85.90	122.0
86.90	2633.0
87.90	2964.0
90.80	418.0
91.90	2147.0
93.00	3084.0
94.00	8602.0
95.00	67320.0
96.00	4697.0
97.00	151.0
103.80	385.0
104.90	108.0
105.80	330.0
106.80	117.0
111.90	135.0
112.90	163.0
115.80	315.0
116.90	604.0
117.70	310.0
118.90	472.0
124.00	103.0
127.90	307.0
128.80	130.0
129.90	367.0
130.90	123.0
134.70	142.0
136.90	196.0
140.90	769.0
141.80	150.0
142.90	764.0
143.80	101.0
145.90	258.0
146.80	115.0
147.80	187.0
148.80	112.0
149.80	145.0
154.90	163.0
156.90	110.0
158.80	125.0
160.90	141.0
168.90	173.0
173.90	50664.0
174.90	3779.0
175.90	48520.0
176.90	3382.0
177.80	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
35.30	130.0
36.00	804.0
37.00	4349.0
38.00	4210.0
39.00	1544.0
40.10	294.0
41.00	168.0
42.00	127.0
43.00	163.0
43.90	1307.0
45.00	1132.0
45.90	132.0
47.00	1022.0
48.00	609.0
49.00	3720.0
50.00	15777.0
51.00	4800.0
52.00	272.0
55.00	251.0
56.00	1399.0
57.00	2609.0
57.90	159.0
59.10	112.0
59.90	743.0
61.00	3985.0
62.00	4070.0
63.00	2979.0
64.00	315.0
64.70	105.0
65.40	133.0
67.00	196.0
68.00	8077.0
69.00	8476.0
70.00	687.0
70.90	102.0
71.90	532.0
73.00	3847.0
74.00	14433.0
75.00	38168.0
76.00	3241.0
76.90	575.0
78.00	406.0
78.90	2672.0
80.00	827.0
80.90	2945.0
81.90	654.0
82.90	124.0
86.00	137.0
86.90	2690.0
87.90	2832.0
90.80	443.0
91.90	2154.0
93.00	3370.0
94.00	8456.0
95.00	69448.0
96.00	4885.0
96.90	170.0
103.80	397.0
104.90	125.0
105.90	426.0
106.90	119.0
111.90	143.0
112.90	191.0
115.80	319.0
116.90	616.0
117.70	310.0
118.90	514.0
127.90	364.0
128.70	161.0
129.90	325.0
131.00	139.0
134.70	186.0
136.90	213.0
140.80	778.0
141.70	193.0
142.90	856.0
145.90	243.0
146.80	128.0
147.80	173.0
149.80	172.0
154.90	160.0
156.90	122.0
158.90	120.0
160.80	135.0
168.90	179.0
173.90	50536.0
174.90	3701.0
175.90	48512.0
176.90	3289.0
177.80	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67