
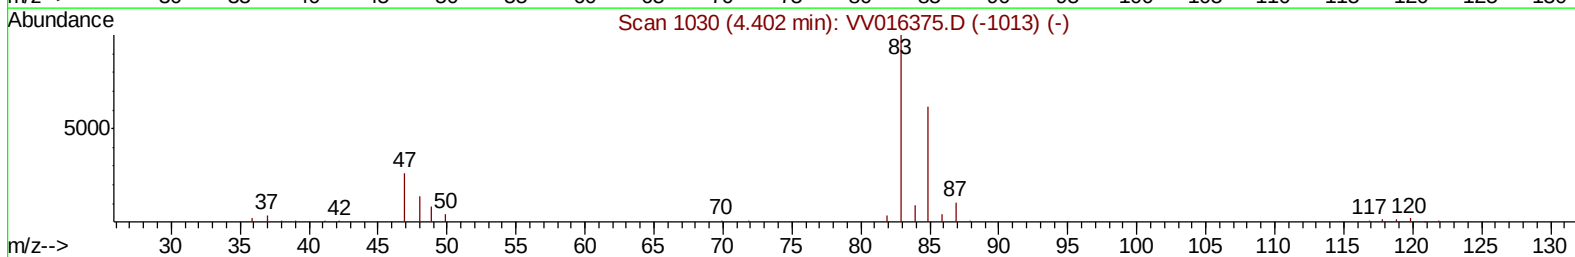
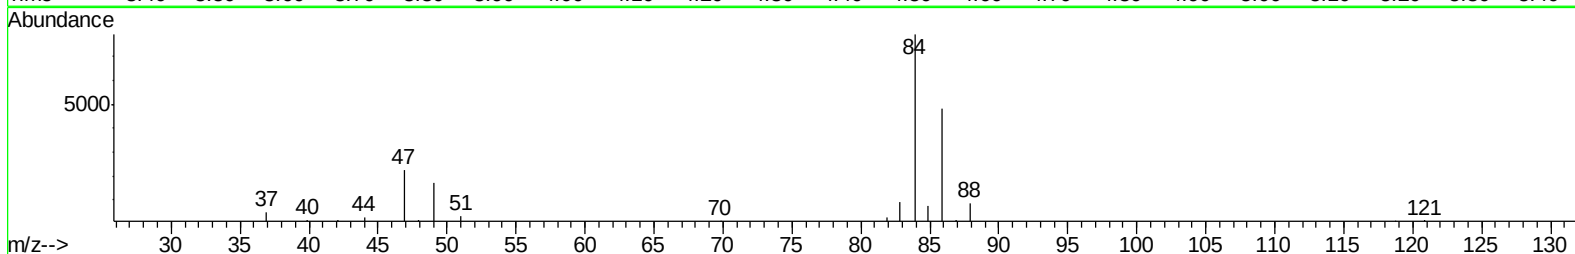


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV053120\
Data File : VV016394.D
Acq On : 31 May 2020 17:50
Operator : SY/MD
Sample : L2780-09
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 01 07:21:18 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 01 07:14:30 2020
Response via : Initial Calibration

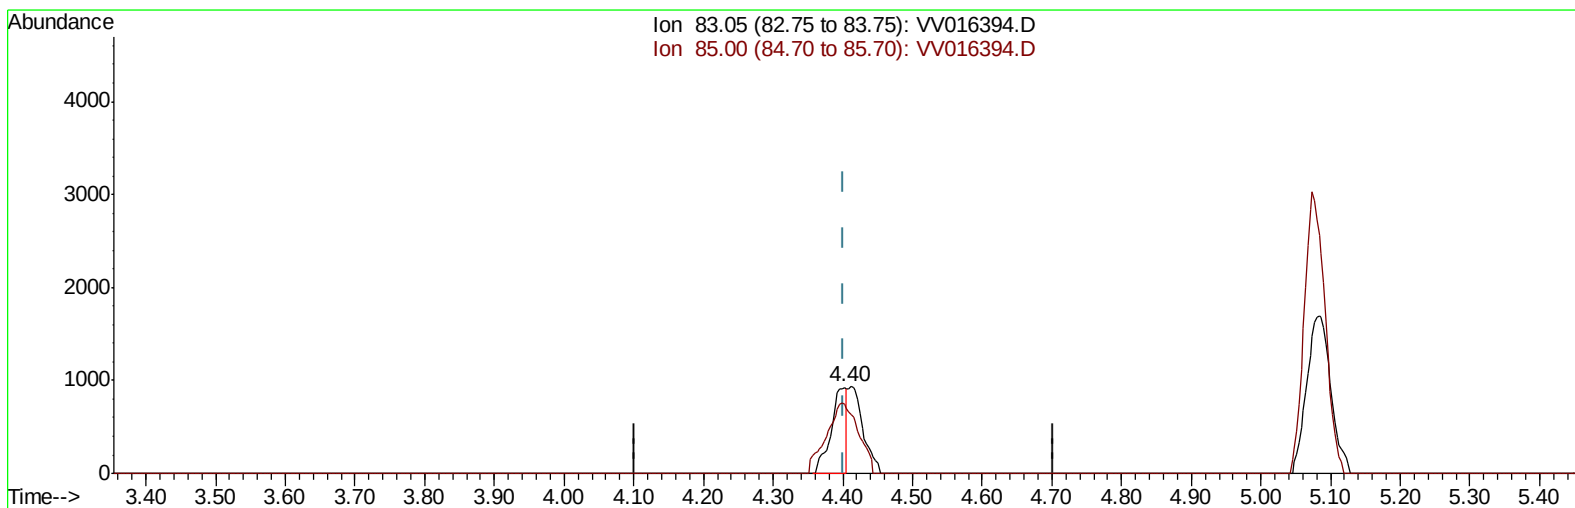

TIC: VV016394.D

(25) Chloroform (T)

4.402min (-0.000) 0.15ug/L

response 1445

Ion	Exp%	Act%
83.05	100	100
85.00	65.50	80.17
0.00	0.00	0.00
0.00	0.00	0.00