

(QT Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV053120\
Data File : VV016383.D
Acq On : 31 May 2020 13:02
Operator : SY/MD
Sample : L2780-04
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM0

Manual Integrations

MMDadoda
6/1/2020 12:44:59 PM

Quant Time: Jun 01 07:54:32 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 01 07:14:30 2020
Response via : Initial Calibration

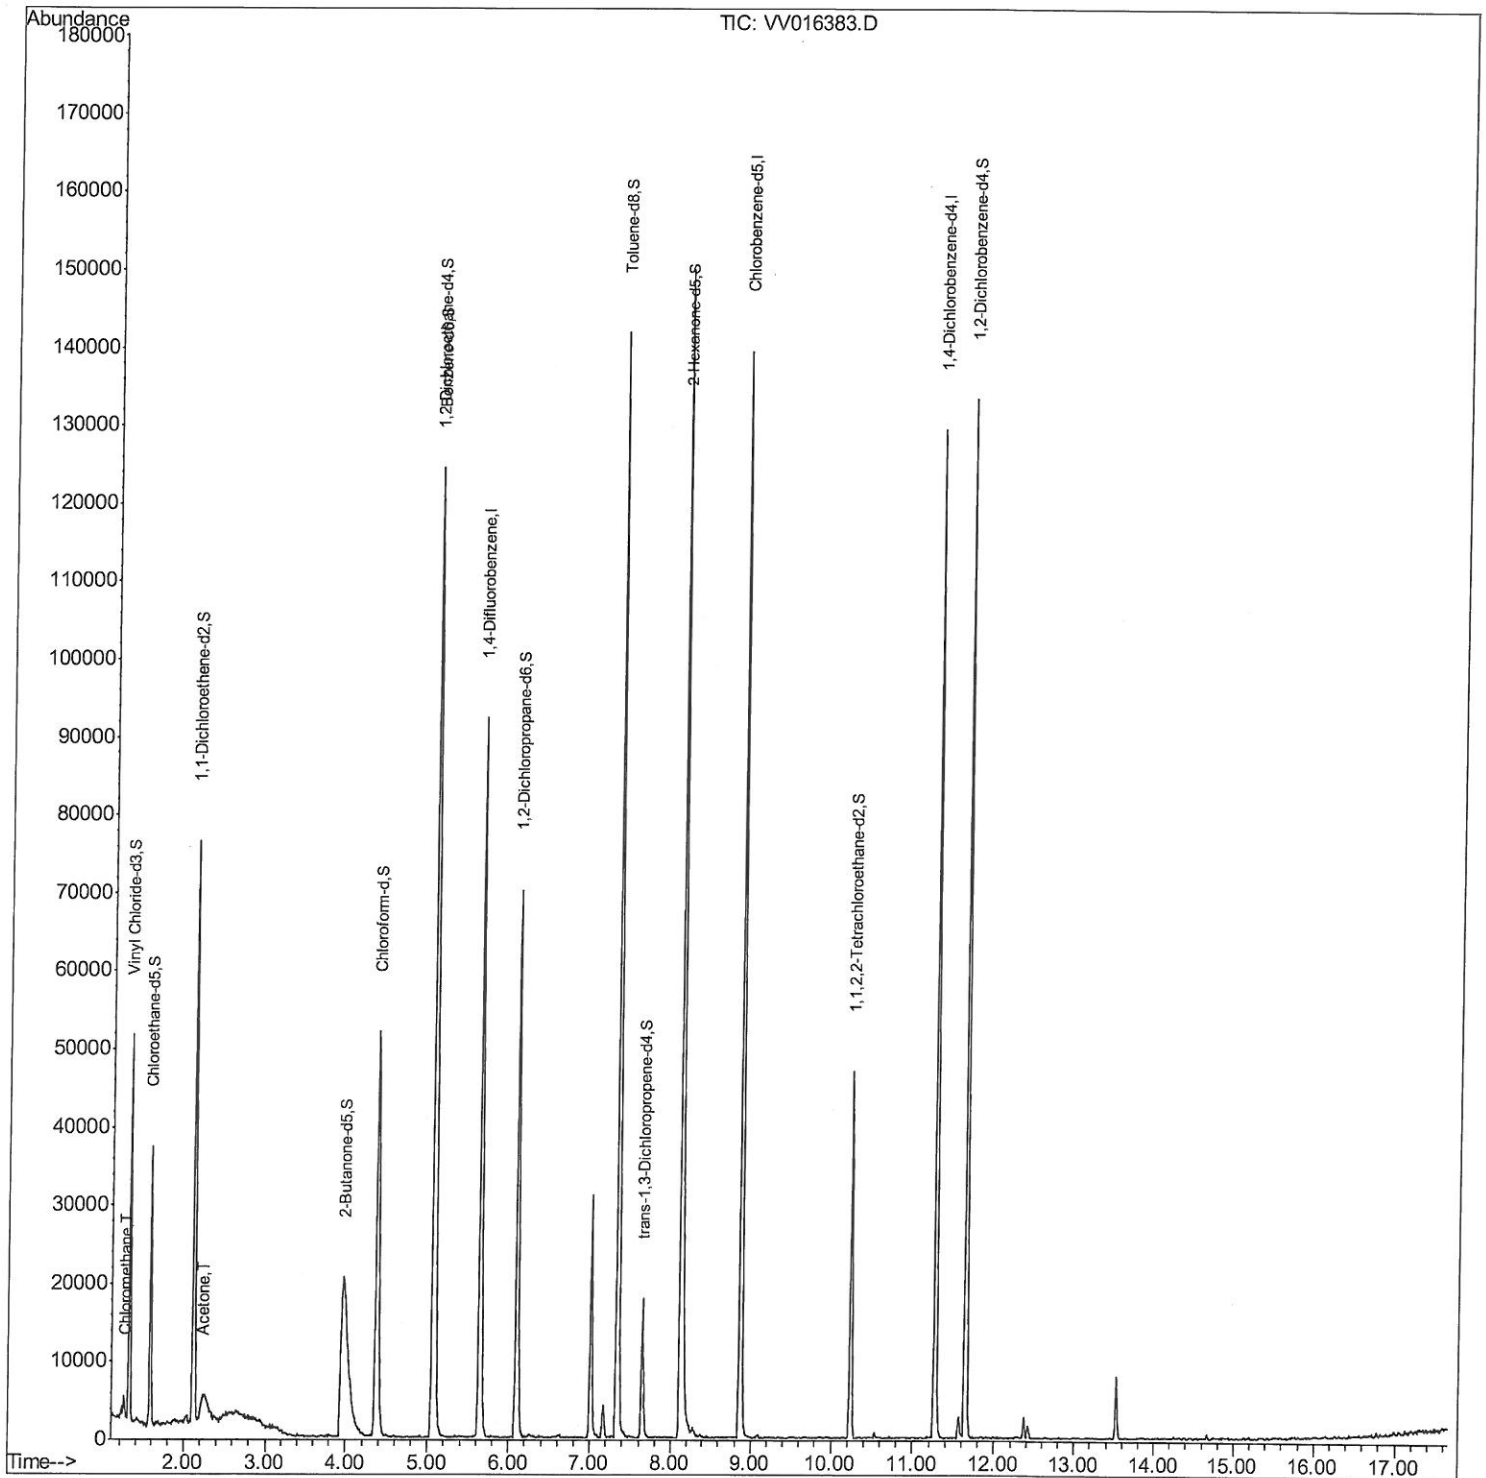

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV053120\
 Data File : VV016383.D
 Acq On : 31 May 2020 13:02
 Operator : SY/MD
 Sample : L2780-04
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampled :
 COAMO

Manual Integrations
APPROVED

MMDadoda
 6/1/2020 12:44:59 PM

Quant Time: Jun 01 07:18:27 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 01 07:14:30 2020
 Response via : Initial Calibration

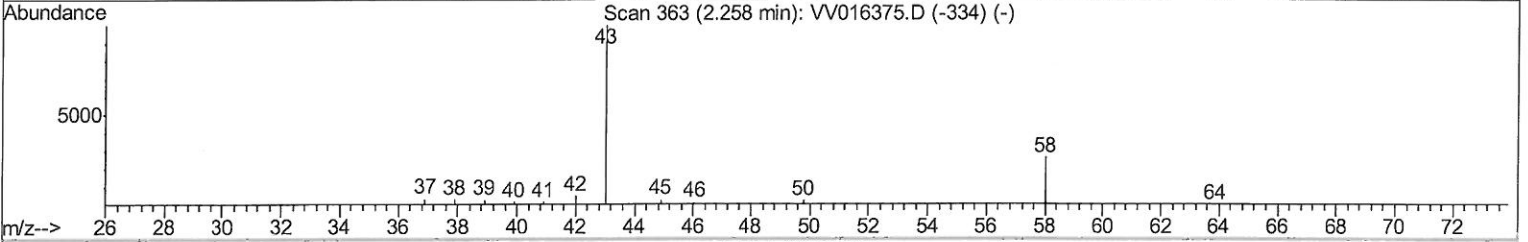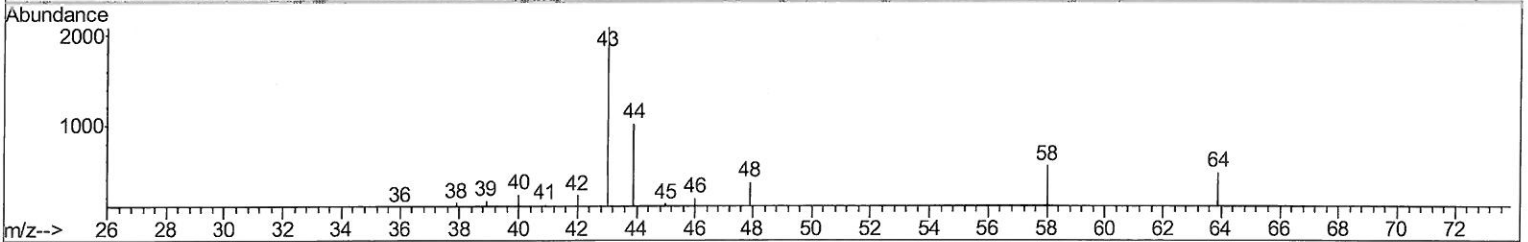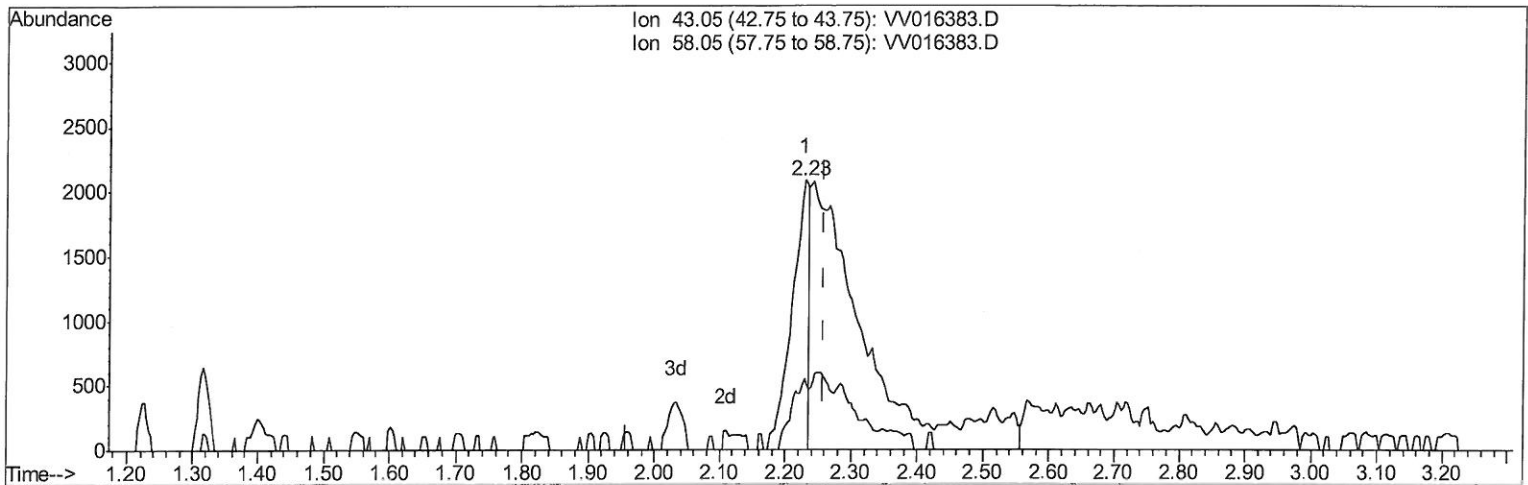

(13) Acetone (T)

2.229min (-0.029) 4.06ug/L

response 3726

Ion	Exp%	Act%
43.05	100	100
58.05	29.60	25.60
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV053120\
 Data File : VV016383.D
 Acq On : 31 May 2020 13:02
 Operator : SY/MD
 Sample : L2780-04
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAMO

Manual Integrations
 APPROVED

MMDadoda
 6/1/2020 12:44:59 PM

Quant Time: Jun 01 07:18:27 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 01 07:14:30 2020
 Response via : Initial Calibration

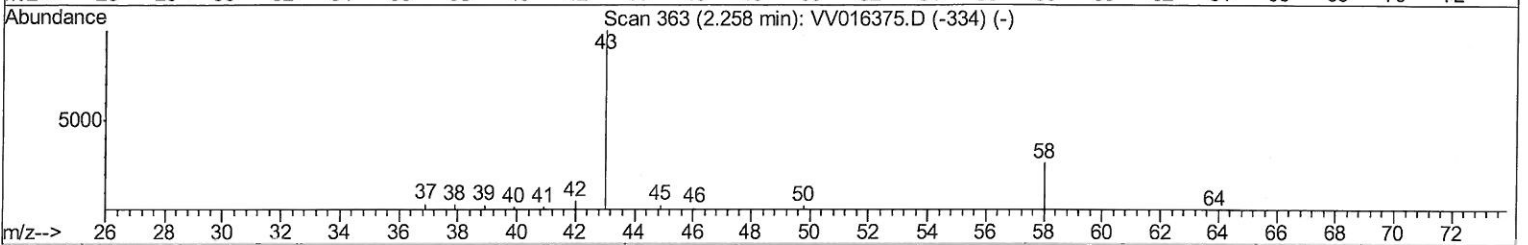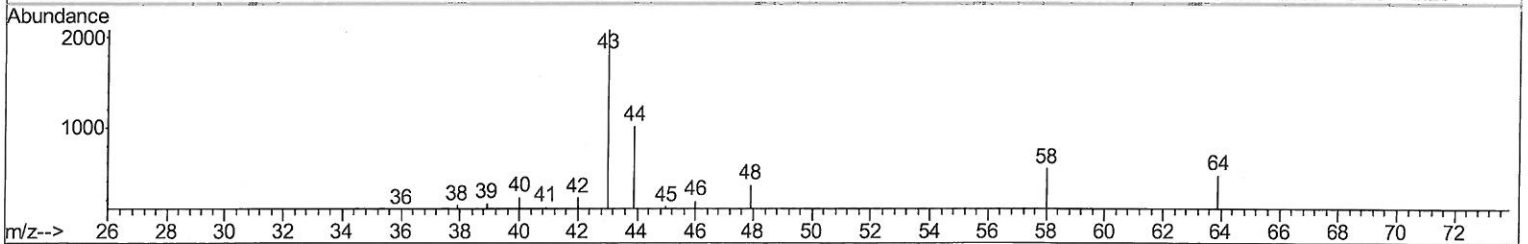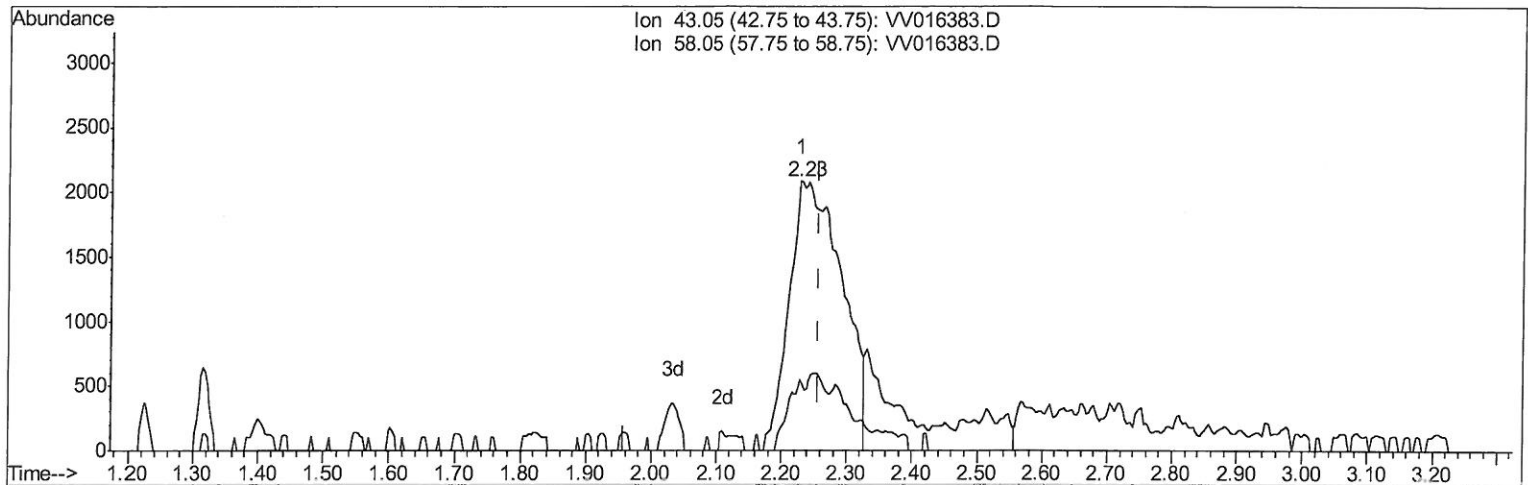

TIC: VV016383.D

(13) Acetone (T)

2.229min (-0.029) 12.75ug/L m

response 11697

Ion	Exp%	Act%
43.05	100	100
58.05	29.60	8.16
0.00	0.00	0.00
0.00	0.00	0.00

MD
 6/02/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV053120\
 Data File : VV016383.D
 Acq On : 31 May 2020 13:02
 Operator : SY/MD
 Sample : L2780-04
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAMO

Manual Integrations
 APPROVED

MMDadoda
 6/1/2020 12:44:59 PM

Quant Time: Jun 01 07:54:32 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 01 07:14:30 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	72211	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	69639	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	29146	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.32	65	29717	4.70	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	94.00%		
7) Chloroethane-d5	1.58	69	23025	4.79	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	95.80%		
11) 1,1-Dichloroethene-d2	2.13	63	40519	3.67	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	73.40%		
20) 2-Butanone-d5	3.96	46	70166	51.44	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	102.88%		
24) Chloroform-d	4.38	84	52167	4.88	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	97.60%		
26) 1,2-Dichloroethane-d4	5.06	65	29078	5.22	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	104.40%		
32) Benzene-d6	5.08	84	102185	5.16	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	103.20%		
36) 1,2-Dichloropropane-d6	6.10	67	31589	5.17	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	103.40%		
41) Toluene-d8	7.34	98	87520	4.84	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	96.80%		
45) trans-1,3-Dichloropropene-	7.65	79	9957	4.52	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	90.40%		
48) 2-Hexanone-d5	8.12	63	50902	49.64	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	99.28%		
59) 1,1,2,2-Tetrachloroethane-	10.24	84	22439	5.20	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	104.00%		
65) 1,2-Dichlorobenzene-d4	11.65	152	29691	5.49	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	109.80%		
Target Compounds						
3) Chloromethane	1.25	50	1611	0.223	ug/L	95
13) Acetone	2.23	43	11697m	12.749	ug/L	7m

(#) = qualifier out of range (m) = manual integration (+) = signals summed

6/02/20