

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV053120\
 Data File : VV016386.D
 Acq On : 31 May 2020 14:14
 Operator : SY/MD
 Sample : L2780-17
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM2

Quant Time: Jun 01 08:02:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 01 07:14:30 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	69799	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	68636	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	29082	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	30102	4.93	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.60%
7) Chloroethane-d5	1.58	69	23641	5.09	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.80%
11) 1,1-Dichloroethene-d2	2.13	63	42271	3.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.20%
20) 2-Butanone-d5	3.95	46	73584	55.81	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.62%
24) Chloroform-d	4.38	84	52362	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.20%
26) 1,2-Dichloroethane-d4	5.06	65	29159	5.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.40%
32) Benzene-d6	5.08	84	103112	5.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.80%
36) 1,2-Dichloropropane-d6	6.10	67	31241	5.19	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.80%
41) Toluene-d8	7.34	98	87786	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.40%
45) trans-1,3-Dichloropropene-	7.65	79	9736	4.48	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.60%
48) 2-Hexanone-d5	8.12	63	50157	49.63	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.26%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	22033	5.18	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.60%
65) 1,2-Dichlorobenzene-d4	11.65	152	30835	5.71	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.20%


Target Compounds					Ovalue
3) Chloromethane	1.25	50	1515	0.217 ug/L	86
13) Acetone	2.21	43	8033	9.058 ug/L	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV053120\
Data File : VV016386.D
Acq On : 31 May 2020 14:14
Operator : SY/MD
Sample : L2780-17
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM2

Quant Time: Jun 01 08:02:47 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 01 07:14:30 2020
Response via : Initial Calibration

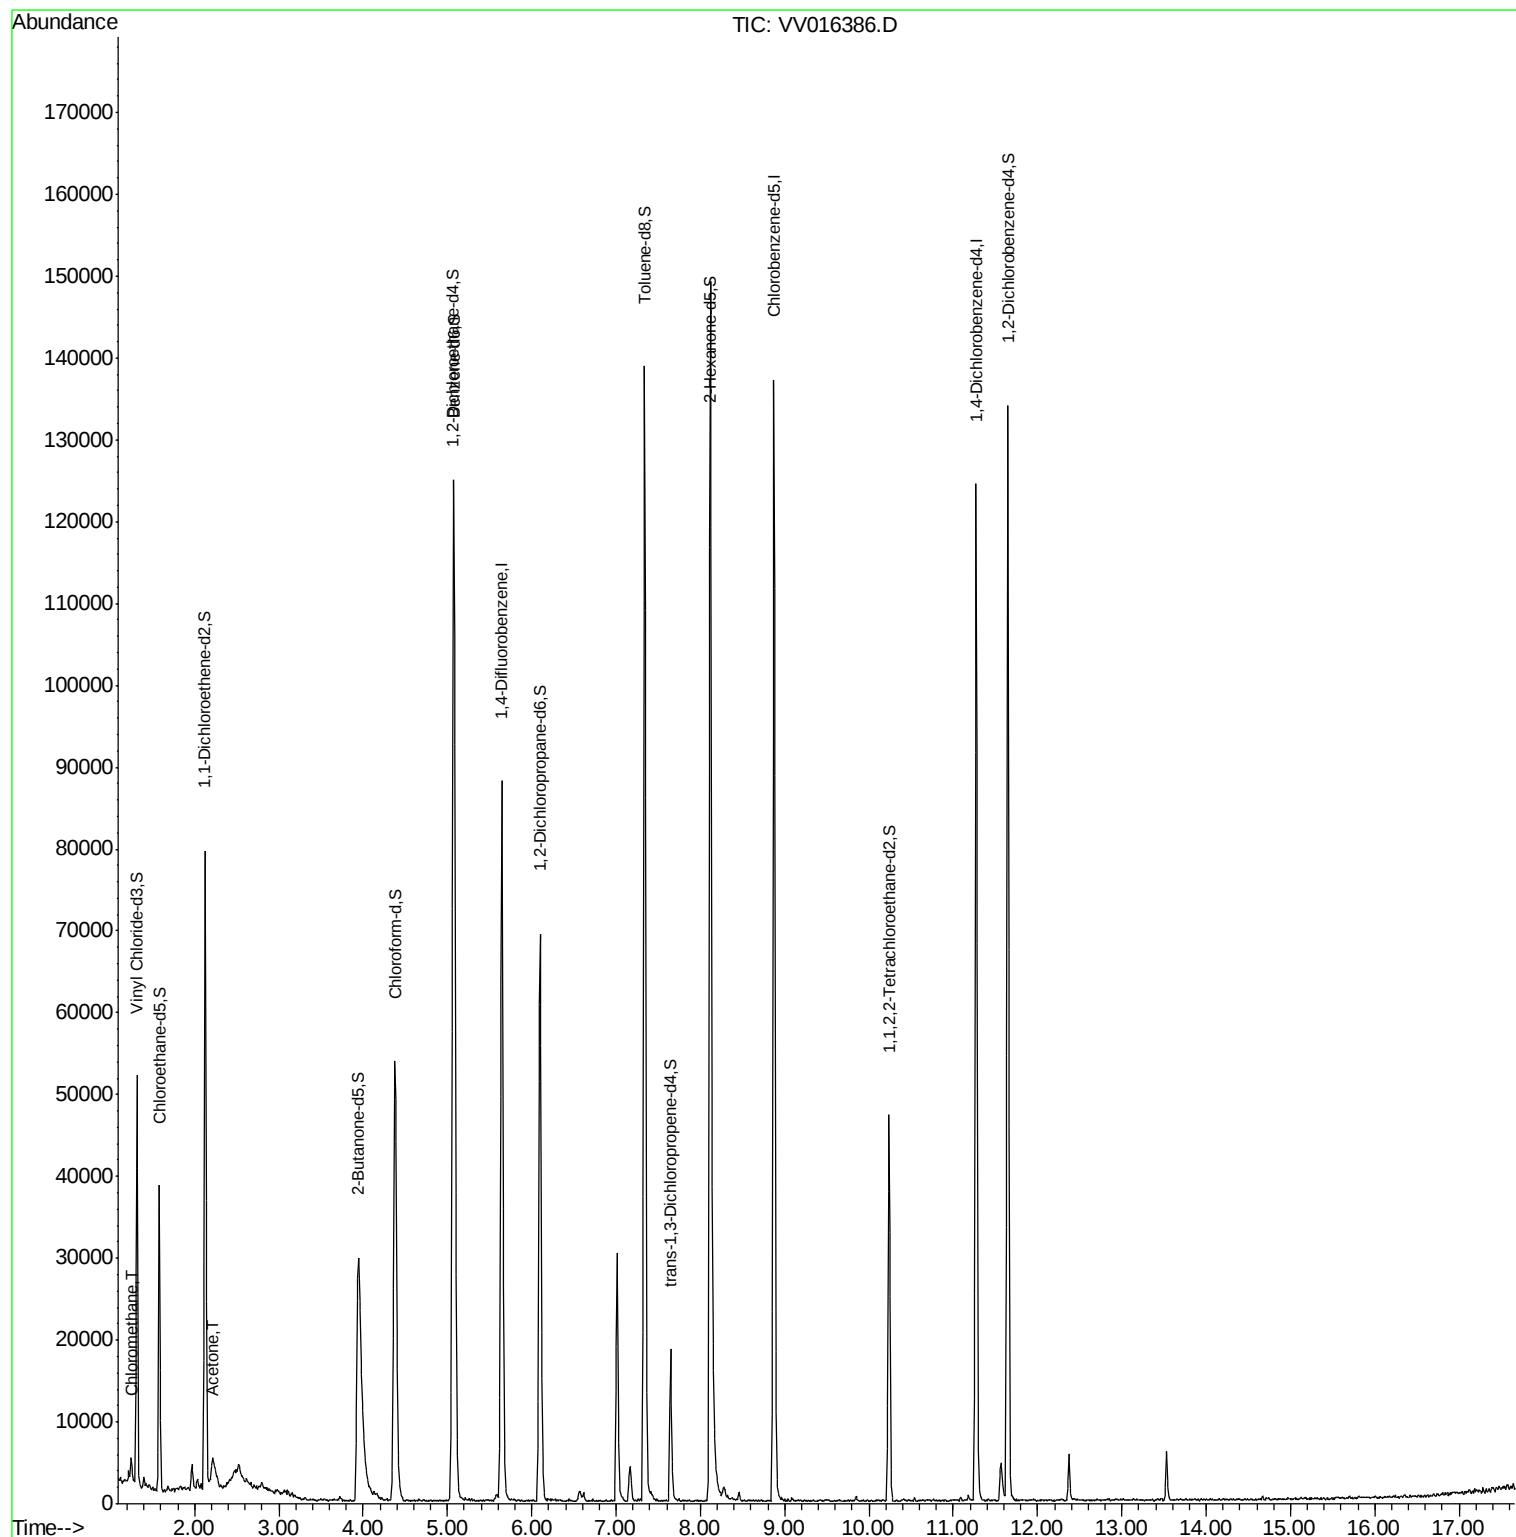

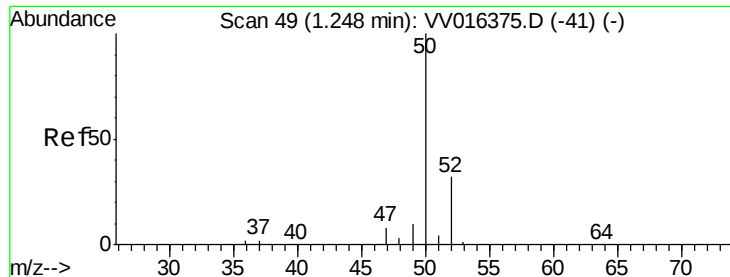

#3

Chloromethane

Concen: 0.217 ug/L

RT: 1.25 min Scan# 50

Delta R.T. 0.00 min

Lab File: VV016386.D

Acq: 31 May 2020 14:14

Instrument :

MSVOA_V

ClientSampleId :


C0AM2

Tot Ion: 50 Resp: 1515

Ion Ratio Lower Upper




50 100

52 40.7 23.1 42.9

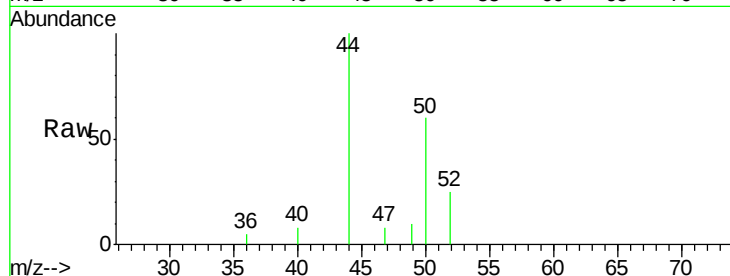

Abundance Ion 50.05 (49.75 to 50.75): VV0

Ion 52.05 (51.75 to 52.75): VV0

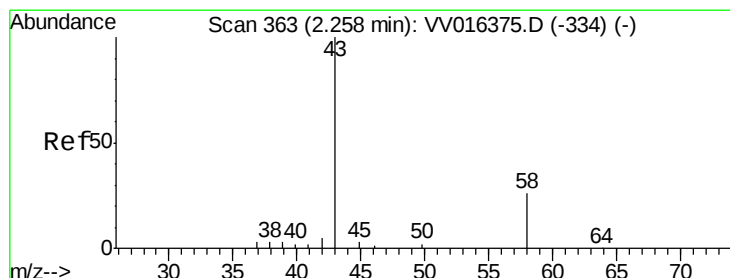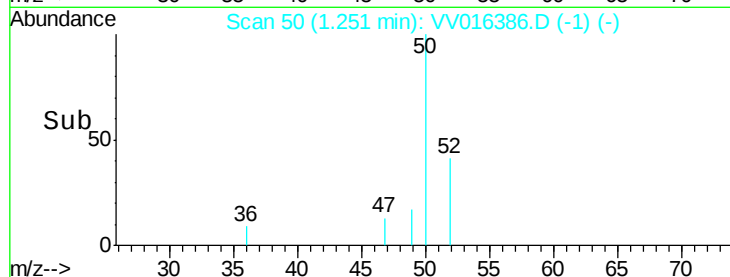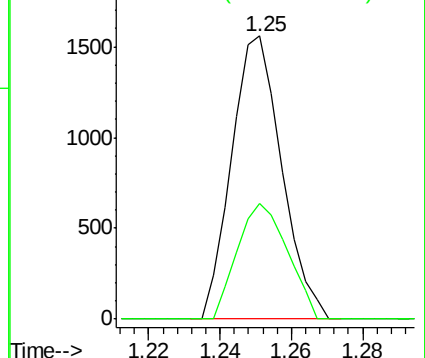

#13

Acetone

Concen: 9.058 ug/L

RT: 2.21 min Scan# 349

Delta R.T. -0.05 min

Lab File: VV016386.D


Acq: 31 May 2020 14:14

Tgt Ion: 43 Resp: 8033

Ion Ratio Lower Upper

43 100

58 16.9 0.0 59.2

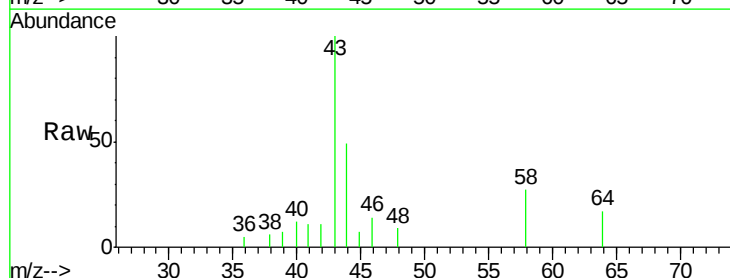

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

